



INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification <sup>6</sup> : <b>G06F 19/00, G01N 21/00</b></p>	<p><b>A1</b></p>	<p>(11) International Publication Number: <b>WO 99/39298</b></p> <p>(43) International Publication Date: 5 August 1999 (05.08.99)</p>														
<p>(21) International Application Number: PCT/US99/02282</p> <p>(22) International Filing Date: 3 February 1999 (03.02.99)</p> <p>(30) Priority Data:</p> <table border="0"> <tr> <td>09/017,901</td> <td>3 February 1998 (03.02.98)</td> <td>US</td> </tr> <tr> <td>09/063,497</td> <td>20 April 1998 (20.04.98)</td> <td>US</td> </tr> </table> <p>(63) Related by Continuation (CON) or Continuation-in-Part (CIP) to Earlier Applications</p> <table border="0"> <tr> <td>US</td> <td>09/063,497 (CIP)</td> </tr> <tr> <td>Filed on</td> <td>20 April 1998 (20.04.98)</td> </tr> <tr> <td>US</td> <td>09/017,901 (CIP)</td> </tr> <tr> <td>Filed on</td> <td>3 February 1998 (03.02.98)</td> </tr> </table> <p>(71) Applicant (for all designated States except US): ADEZA BIOMEDICAL CORPORATION [US/US]; 1240 Elko Drive, Sunnyvale, CA 94089 (US).</p> <p>(72) Inventors; and</p> <p>(75) Inventors/Applicants (for US only): ANDERSON, Emory, V. [US/US]; 2105 Canyon Oak Lane, Danville, CA 94506 (US). LAPOINTE, Jerome [US/US]; 6120 Bullard Drive, Oakland, CA 94611 (US). MARTINEZ, Ricardo [US/US]; 110 Tree Frog Lane, Santa Cruz, CA 95060 (US). MAR-</p>		09/017,901	3 February 1998 (03.02.98)	US	09/063,497	20 April 1998 (20.04.98)	US	US	09/063,497 (CIP)	Filed on	20 April 1998 (20.04.98)	US	09/017,901 (CIP)	Filed on	3 February 1998 (03.02.98)	<p>ZOLF, Gail [US/US]; 1138 Kentwood Avenue, Cupertino, CA 95014 (US). PONG, Ronald [US/US]; 4935 Palacewood Court, San Jose, CA 95129 (US). JONES, Lynn [US/US]; 13175 Franklin Avenue, Mountain View, CA 94040 (US). HUSSA, Robert, O. [US/US]; 1164-A La Rochelle Terrace, Sunnyvale, CA 94089 (US). NEMEC, Edward [US/US]; 3560 Stateloy Oaks Lane, Duluth, GA 30097 (US). SENYEI, Andrew [US/US]; 1740 El Camino del Teatro, La Jolla, CA 92037 (US). DESIENO, Duane, D. [US/US]; 2015 Olite Court, La Jolla, CA 92037 (US).</p> <p>(74) Agent: SEIDMAN, Stephanie, L.; Heller Ehrman White &amp; McAuliffe, Suite 700, 4250 Executive Square, La Jolla, CA 92037 (US).</p> <p>(81) Designated States: AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, CA, CH, CN, CU, CZ, DE, DK, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MD, MG, MK, MN, MW, MX, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, UA, UG, US, UZ, VN, YU, ZW, ARIPO patent (GH, GM, KE, LS, MW, SD, SZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).</p> <p><b>Published</b> With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</p>
09/017,901	3 February 1998 (03.02.98)	US														
09/063,497	20 April 1998 (20.04.98)	US														
US	09/063,497 (CIP)															
Filed on	20 April 1998 (20.04.98)															
US	09/017,901 (CIP)															
Filed on	3 February 1998 (03.02.98)															
<p>(54) Title: POINT OF CARE DIAGNOSTIC SYSTEMS</p> <p>(57) Abstract</p> <p>Systems and methods for medical diagnosis or risk assessment for a patient are provided. These systems and methods are designed to be employed at the point of care, such as in emergency rooms and operating rooms, or in any situation in which a rapid and accurate result is desired. The systems and methods process patient data, particularly data from point of care diagnostic tests or assays, including immunoassays, electrocardiograms, X-rays and other such tests, and provide an indication of a medical condition or risk or absence thereof. The systems include an instrument for reading or evaluating the test data and software for converting the data into diagnostic or risk assessment information.</p>																

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AL	Albania	ES	Spain	LS	Lesotho	SI	Slovenia
AM	Armenia	FI	Finland	LT	Lithuania	SK	Slovakia
AT	Austria	FR	France	LU	Luxembourg	SN	Senegal
AU	Australia	GA	Gabon	LV	Latvia	SZ	Swaziland
AZ	Azerbaijan	GB	United Kingdom	MC	Monaco	TD	Chad
BA	Bosnia and Herzegovina	GE	Georgia	MD	Republic of Moldova	TG	Togo
BB	Barbados	GH	Ghana	MG	Madagascar	TJ	Tajikistan
BE	Belgium	GN	Guinea	MK	The former Yugoslav Republic of Macedonia	TM	Turkmenistan
BF	Burkina Faso	GR	Greece	ML	Mali	TR	Turkey
BG	Bulgaria	HU	Hungary	MN	Mongolia	TT	Trinidad and Tobago
BJ	Benin	IE	Ireland	MR	Mauritania	UA	Ukraine
BR	Brazil	IL	Israel	MW	Malawi	UG	Uganda
BY	Belarus	IS	Iceland	MX	Mexico	US	United States of America
CA	Canada	IT	Italy	NE	Niger	UZ	Uzbekistan
CF	Central African Republic	JP	Japan	NL	Netherlands	VN	Viet Nam
CG	Congo	KE	Kenya	NO	Norway	YU	Yugoslavia
CH	Switzerland	KG	Kyrgyzstan	NZ	New Zealand	ZW	Zimbabwe
CI	Côte d'Ivoire	KP	Democratic People's Republic of Korea	PL	Poland		
CM	Cameroon	KR	Republic of Korea	PT	Portugal		
CN	China	KZ	Kazakstan	RO	Romania		
CU	Cuba	LC	Saint Lucia	RU	Russian Federation		
CZ	Czech Republic	LI	Liechtenstein	SD	Sudan		
DE	Germany	LK	Sri Lanka	SE	Sweden		
DK	Denmark	LR	Liberia	SG	Singapore		
EE	Estonia						

**POINT OF CARE DIAGNOSTIC SYSTEMS****RELATED APPLICATIONS**

This application claims the benefit of priority to U.S. application Serial No. 09/063,497, filed April 20, 1998, to Emory V. Anderson, Edward Nemec,  
5 Jerome Lapointe, Duane DeSieno, Ricardo Martinez, Gail Marzolf, Ronald Pong, Lynn Jones, Robert O. Husa and Andrew Senyei, entitled "POINT OF CARE DIAGNOSTIC SYSTEMS, and to U.S. application Serial No. 09/017,901, filed February 3, 1998 to Emory V. Anderson, Edward Nemec, Jerome Lapointe, Duane DeSieno, Ricardo Martinez, Gail Marzolf, Ronald Pong, Lynn Jones,  
10 Robert O. Husa and Andrew Senyei, entitled "POINT OF CARE DIAGNOSTIC SYSTEMS." For purposes of the United States, this application is a continuation-in-part of the above-identified applications.

This application is also related to U.S. application Serial No. 08/599,275 to Jerome Lapointe and Duane DeSieno, filed February 9, 1996, entitled  
15 "METHOD FOR DEVELOPING MEDICAL AND BIOCHEMICAL DIAGNOSTIC TESTS USING NEURAL NETWORKS", now abandoned, copending U.S. application Serial No. 08/798,306 to Jerome Lapointe and Duane DeSieno, filed February 7, 1997, entitled "METHOD FOR SELECTING MEDICAL AND BIOCHEMICAL DIAGNOSTIC TESTS USING NEURAL NETWORK-RELATED  
20 APPLICATIONS", and copending U.S. application Serial No. 08/912,133 to Jerome Lapointe and Duane DeSieno, filed August 14, 1997, entitled "METHOD FOR SELECTING MEDICAL AND BIOCHEMICAL DIAGNOSTIC TESTS USING NEURAL NETWORK-RELATED APPLICATIONS"; and also copending U.S. application Serial No. 09/134,636, filed August 14, 1998. The subject matter  
25 of these applications is also described in International PCT application Nos. WO 97/29447 and PCT/US98/16891.

Where permitted, the subject matter of each of these patents and each of U.S. Application Serial Nos. 09/017,901, 08/599,275, 08/798,306 and 08/912,133 is herein incorporated herein by reference in its entirety. The

-2-

subject matter of published International PCT application No. International PCT application No. WO 97/29447, which corresponds to U.S. application Serial No. 08/912,133 is also herein incorporated in its entirety by reference thereto. U.S. Design Patent Applications Serial Nos. 29/086781 and 29/086799, each filed  
5 April 20, 1998, are also incorporated by reference herein.

#### **FIELD OF THE INVENTION**

The present invention relates to systems and methods that aid in providing a medical diagnosis or risk assessment for a patient using biochemical and historic patient data, including data from point of care diagnostic tests or  
10 assays, and processing the information to give an indication of a medical condition or risk.

#### **BACKGROUND OF THE INVENTION**

##### **Evaluation of Immunoassay Data**

In diagnostic immunochromatographic assays, where results are  
15 determined by a color change or the production of color, results are generally detected visually by human eye. As a result of the human perception and judgment involved, there is significant variance among those interpreting such test results as to whether a color change or other measurable signal has occurred, and the degree of such occurrence. Furthermore, there is a great deal  
20 of subjectivity involved in interpreting whether immunoassay results are positive or negative. This is particularly pronounced where the result is close to a threshold value. The variance is further enhanced when attempts are made to quantitate such assay test results. Accurate results may be critical for certain diagnostic assays.

25 It is desirable to develop techniques that are objective in nature, and that reduce the error associated with interpreting immunochromatographic and other assay test results. Therefore, it is an object herein to provide systems, methods, devices and instruments for objectively assessing data from biochemical and other tests and to use such data for diagnosis and risk  
30 assessment. It is also an object herein to incorporate decision-support methodologies into such systems and thereby enhance the diagnostic and risk assessment capabilities thereof.

-3-

It is also an object herein to provide systems and methods for use in detecting and measuring fetal fibronectin (fFN) levels in a patient sample and using such information to diagnose and assess risks of preterm labor, fetal membrane rupture and other related disorders and conditions of concern during pregnancy that may comprise the pregnancy or harm the newborn, including, for example, ascending genital infections such as chlamydia or herpes simplex virus.

#### SUMMARY OF THE INVENTION

Systems and methods for medical diagnosis or risk assessment for a patient are provided. These systems and methods are designed to be employed at the point of care, such as in emergency rooms, operating rooms, hospital laboratories and other clinical laboratories, doctor's offices, in the field, or in any situation in which a rapid and accurate result is desired. The systems and methods process patient data, particularly data from point of care diagnostic tests or assays, including immunoassays, chemical assays, nucleic acid assays, colorimetric assays, fluorometric assays, chemiluminescent and bioluminescent assays, electrocardiograms, X-rays and other such tests, and provide an indication of a medical condition or risk or absence thereof.

The systems include an instrument for reading or evaluating the test data and software for converting the data into diagnostic or risk assessment information. In certain embodiments, the systems include a test device, such as a test strip, optionally encased in a housing, for analyzing patient samples and obtaining patient data. In particular embodiments, the device includes a symbology, such as a bar code, which is used to associate identifying information, such as intensity value, standard curves, patient information, reagent information and other such information, with the test device. The reader in the system is optionally adapted to read the symbology.

Further, the systems optionally include a decision-support system or systems, such as a neural network, for evaluating the data, and also for subsequent assessment of the data, such as by integration with other patient information, including documents and information in medical records. All software and instrument components are preferably included in a single

-4-

package. Alternatively, the software can be contained in a remote computer so that the test data obtained at a point of care can be sent electronically to a processing center for evaluation.

The patient information includes data from physical and biochemical tests, such as immunoassays, and from other procedures. The test is performed on a patient at the point of care and generates data that can be digitized, such as by an electronic reflectance or transmission reader, which generates a data signal. The signal is processed using software employing data reduction and curve fitting algorithms, or a decision support system, such as a trained neural network, or combinations thereof, for converting the signal into data, which is used to aid in diagnosis of a medical condition or determination of a risk of disease. This result may be further entered into a second decision support system, such as a neural net, for refinement or enhancement of the assessment.

In a particular embodiment, systems and methods for detecting and measuring levels of a target analyte in a patient sample, analyzing the resulting data, and providing a diagnosis or risk assessment are provided. The systems and methods include an assay device in combination with a reader, particularly a computer-assisted reader, preferably a reflectance reader, and data processing software, preferably employing data reduction and curve fitting algorithms, optionally in combination with a trained neural network, for accurately determining the presence or concentration of analyte in a biological sample. In a preferred embodiment, the methods include the steps of performing an assay on a patient sample, reading the data using a reflectance reader and processing the reflectance data using data processing software. In a particular embodiment, the assay is an immunoassay. Preferred software includes data processing software employing data reduction and curve fitting algorithms, optionally in combination with a trained neural network, to determine the presence or amount of analyte in a given sample. The data obtained from the reader then can be further processed by the medical diagnosis system to provide a risk assessment or diagnosis of a medical condition as output. In alternative embodiments, the output can be used as input into a subsequent

-5-

decision support system, such as a neural network, that is trained to evaluate such data.

In a preferred embodiment, the assay device is a lateral flow test strip, preferably, though not necessarily, encased in a housing, designed to be read by the reader, and the assay is a sandwich immunoassay. For example, in one embodiment thereof, a patient sample is contacted with an antibody for a selected target analyte indicative of a disease, disorder or risk thereof. The antibody is preferably labeled by conjugation to a physically detectable label, and upon contacting with the sample containing the target analyte forms a complex. The antibody-analyte complex is then contacted with a second antibody for the antigen, which is immobilized on a solid support. The second antibody captures the antibody-analyte complex to form an antibody-analyte-antibody sandwich complex, and the resulting complex, which is immobilized on the solid support, is detectable by virtue of the label. The test strip is then inserted into a reader, where the signal from the label in the complex is measured. Alternatively, the test strip could be inserted into the reader prior to addition of the sample. Additionally, the housing may include a symbology, such as a bar code, which is also read by the reader and contains data related to the assay device and/or test run. The signal obtained is processed using data processing software, preferably employing data reduction and curve fitting algorithms, optionally in combination with a trained neural network, to give either a positive or negative result, or a quantitative determination of the concentration of analyte in the sample, which is correlated with a result indicative of a risk or presence of a disease or disorder. This result can optionally be input into a decision support system, and processed to provide an enhanced assessment of the risk of a medical condition as output. The entire procedure may be automated and/or computer-controlled.

In certain embodiments, the reflectance reader is adapted to read a symbology on the test device. The symbology is preferably a bar code, which be read in the same manner that the test strip in the device can be read. In these embodiments, the reader head scans across a bar code in a stepwise fashion. The data collected from the bar code is transformed into integrated

-6-

peak information and analyzed as alphanumeric characters, which are related to information related to the particular device and/or test run or other information, including patient information. Any bar code from among the many known in the in industry. In preferred embodiments, Code 39 (a trademark of Interface Mechanism, Inc., Lynnwood, WA; see, e.g., U.S. Patent No. 4,379,224, U.S. Patent No. 4,438,327, U.S. Patent No. 4,511,259 or Code 128 bar codes (see, e.g., U.S. Patent No. 5,227,893) are used.

In a particular embodiment, the analyte to be detected is fetal fibronectin (fFN) and the result obtained is a positive or negative indication of pregnancy or the risk of certain pregnancy-related conditions or fertility and infertility-related conditions, including ectopic pregnancy, preterm labor, pre-eclampsia, imminent delivery, term induction and fetal membrane rupture and infections of concern during pregnancy that may comprise the pregnancy or harm the newborn, including, for example, ascending genital infections such as chlamydia or herpes simplex virus. Thus, provided herein is a rapid fFN test using a lateral flow test device.

At the very least, this test provides the same clinically relevant information as a fFN ELISA (an enzyme linked immunosorbent sandwich assay (ELISA)) test heretofore available in significantly less time and at the point of care. The fFN immunoassay provided herein allows the user to test a cervicovaginal swab sample in about 20 minutes. When practiced as described herein, additional information, such as a more accurate risk assessment or diagnosis, can be obtained.

The system herein provides a means to detect and to quantitate concentrations of fFN throughout pregnancy and to assess the risk and detect conditions associated therewith. Because of the sensitivity of the combination of the reader and devices provided herein, fFN may be monitored throughout pregnancy, including times when it is not detected by less sensitive systems.

The reflectance reader and test strip device are also provided herein. Also provided herein are the neural nets for assessing the data.



-7-

A method for classifying an image is also provided. The method includes the steps of reducing the image to a set of derived parameters from which the image can be reconstructed within a predetermined degree of tolerance; inputting the derived parameters into a classification neural network; and

5 determining the classification of the image based on the output of the classification neural network. The method of reducing the image to a set of derived parameters is achieved by defining a mathematical function that contains a plurality of parameters representative of the image; and optimizing the parameters of the function using a methodology that minimizes the error

10 between the image and a reconstruction of the image using the function.

In an alternative embodiment, the method of reducing the image to a set of derived parameters is achieved by inputting the image into a trained neural network, where the inputs to the network represent the image, the hidden layer of the network is such that the number of hidden elements is smaller than the

15 number of inputs to the network, and the outputs of the network represent reconstruction of the image; and setting the derived parameters to the output values of the trained neural network.

In another alternative embodiment, the method of reducing the image to a set of derived parameters is achieved by defining a neural network in which

20 the inputs to the network are the coordinates of a point in the image, the hidden layer contains a plurality of elements, and the output of the network represents the reconstruction of the associated point in the image; training the neural network so that the error between the network output and the image are minimized for all points in the image; and setting the derived parameters to the

25 weights of the hidden layer of the trained neural network.

The neural networks and computer systems used in the methods are also provided.

Also provided are methods for assessing the validity of diagnostic test results and for a method for developing controls for assays. The method of

30 developing a control for any assay system includes the steps of analyzing a plurality of test runs of the assay and obtaining results of the test runs;

-8-

classifying the results by type of result; and identifying a pattern representative of or predictive of each type of result. When the assay is run the results therefrom are compared to the representative pattern, and, if the results vary from the pattern, they can be discarded. The pattern and classification can be  
5 effected by any decision support system, including curve fitting routines and neural nets. For example, data from an assay are fit to to a predetermined curve based on expected results for a predetermined number of iterations. If the curve for a particular run of the assay deviates beyond an acceptable predetermined fit, the data from the assay is rejected. The curve data can be  
10 generated for any type of test and typically will encompass at least variables. For example, for the fFN assay provided herein a curve or function for intensity of the reading versus the distance traveled on the strip (generally normalized) has been generated based on numerous runs of the assay. For any given run of the assay, if the curve of intensity versus distance varies by a selected  
15 predetermined amount, it indicates that the assay did not run properly, and the results should be discarded. If the results match the curve, then this indicates that the assay ran properly. This type of curve fitting can be performed for any assay or test and can use typically at least two and up to any number of variables or parameters for generating the curve. This may generated and the  
20 control step performed using a neural network or other decision support system.

#### **BRIEF DESCRIPTION OF THE DRAWINGS**

FIG. 1A is a top view of an assay test strip, such as an immunoassay test strip;

FIG. 1B is a side view of the assay test strip of FIG. 1;

25 FIG. 2A is a perspective view of an assay device, including the assay test strip of FIG. 1A and FIG. 1B and housing assembly and showing a bar code, which can optionally be affixed to the housing;

FIG. 2B is a perspective view of an alternative embodiment of an assay device, including the assay test strip of FIG. 1A and FIG. 1B and housing  
30 assembly and showing a bar code, which can optionally be affixed to the housing;

FIG. 3 is a perspective view of the assay device of FIG. 2B showing the individual components of the device;

FIG. 4 is a top view of an exemplary housing assembly for the assay test strip of FIG. 1;

5       FIG. 5 is a side assembly view of the housing assembly of FIG. 4;

FIG. 6 is a top view of an embodiment of an assay reader and an assay device, inserted therein, in accordance with an exemplary embodiment of the reader;

10       FIG. 7 is a perspective view of portion of the assay device of FIG. 2A shown inserted into a cassette slot of a lower housing and extending to a reader head assembly within an exemplary embodiment of an assay reader;

FIG. 8 is a top view of the lower housing of the assay reader of FIG. 7 with the assay device inserted therein and a stepper motor shown positioned relative to the assay device as is when the assay device is fully inserted into the  
15       cassette slot of the reader;

FIG. 9 is a side view of the lower housing of the reader device of FIG. 7 with the assay device of FIG. 2A fully inserted with the stepper motor shown positioned relative to the fully inserted assay device, with a reader head shown positioned in a lowered position over a test opening of the assay device, and  
20       with a carriage wheel shown engaged by the assay device so as to lower the reader head into its lowered position therein;

FIG. 10 is a side view of a reader head assembly such as is found in the reader device of FIG. 6;

FIG. 11 is a side view of a reader head of the reader head assembly of  
25       FIG. 10;

FIG. 12 is a reverse angle side view of the reader head assembly of FIG. 10;

FIG. 13 is a reverse angle side view of the reader head of FIG. 11;

FIG. 14 is a side view of the reader head assembly of FIG. 10, having  
30       been actuated so as to pivot the reader head assembly into a raised position suitable for insertion and removal of the assay device into and from the reader head assembly within the assay reader;

-10-

FIG. 15 is an end view of the reader head of FIG. 11;

FIG. 16 is an end view of the reader head assembly of FIG. 10;

FIG. 17 is a cut-away view of the reader head assembly of FIG. 11 with first and second light emitting diodes, a photodetector, corresponding fiberoptic bundles and an aperture at a lower end thereof depicted;

FIG. 18 is a partial closeup cross-sectional view of a reader head tip of the reader head of FIG. 17 showing the aperture and ends of fiberoptic fibers of the fiberoptic bundles of FIG. 17;

FIG. 19 is a closeup bottom view of the aperture of the reader head of FIG's. 17 and 18 illustrating a sigmoidal pattern for positioning individual fiberoptic fibers (fiberoptic conductors);

FIG. 20 is a closeup end view of the corresponding fiberoptic bundle at the first light emitting diode of FIG. 17 from which the fiberoptic bundle conducts light from the first light emitting diode;

FIG. 21 is a schematic diagram illustrating a process by which an assay test strip is analyzed so as to determine an amount of background light at a control region of the assay test strip;

FIG. 22 is a schematic diagram illustrating a process by which an assay test strip is analyzed so as to determine an amount of reflection resulting from a first illumination of a control portion of the assay test strip; and

FIG. 23 is a schematic view diagram illustrating a process by which an assay test strip is analyzed so as to determine an amount of reflection resulting from a second illumination of a control portion of the assay test strip;

FIG. 24 is a side view of an exemplary embodiment of the reader that is adapted for reading a bar code; and

FIG. 25 is an example of a bar code in accordance with an exemplary embodiment of the assay device.

## **DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS**

### **Definitions**

Unless defined otherwise, all technical and scientific terms used herein have the same meaning as is commonly understood by one of skill in the art to which this invention belongs. All patents and publications referred to herein

-11-

are, unless noted otherwise, incorporated by reference in their entirety. In the event a definition in this section is not consistent with definitions elsewhere, the definition set forth in this section will control.

As used herein, point of care testing refers to real time diagnostic testing  
5 that can be done in a rapid time frame so that the resulting test is performed faster than comparable tests that do not employ this system. For example, the exemplified fFN immunoassay, is performed in less time than the fFN ELISA assay (i.e., less than about 3 to 4 hours, preferably less than 1 hour, more preferably less than half an hour). In addition, with the method and devices  
10 provided herein, it can be performed rapidly and on site, such as in a doctor's office, at a bedside, in a stat laboratory, emergency room or other such locales, particularly where rapid and accurate results are required. The patient can be present, but such presence is not required. Point of care includes, but is not limited to: emergency rooms, operating rooms, hospital laboratories and other  
15 clinical laboratories, doctor's offices, in the field, or in any situation in which a rapid and accurate result is desired.

As used herein, an anti-fFN antibody is an antibody that binds selectively with fFN. Such antibodies are known to those of skill in the art and also may be readily isolated.

20 As used herein, a test strip refers to any means on which patient test data or other data is generated, recorded or displayed in a manner that forms an image or from which an image can be generated. Such strips, include, but are not limited to, immunochromatographic test strips, such as lateral flow devices, X-ray films, such as X-rays and films produced from sequencing gels, EKG  
25 printouts, MRI results and other such means that generate or from which an image as defined herein can be generated. The strip is preferably adapted for scanning or reading by a reader, preferably the reader provided herein. Although referred to as a "strip", it can be of any shape or geometry, including rectangular, three dimensional, circular, and so forth.

30 As used herein, a sigmoidal pattern (also referred to herein as sigmoidal-like; see, e.g., FIG. 19) with reference to the fiberoptics refers to the S-shaped or snake-like pattern of illumination selected for maximizing illumination across

-12-

the lines on the test strip. The pattern is not strictly a sigmoidal shape, but refers to a pattern such as that depicted in FIG. 19, which pattern provides a means for adding more area to any reading. Any other pattern that achieved this result is encompassed within this expression.

5           As used herein, quantitative results are results that are absolute or relative values; qualitative results are typically negative or positive type results.

          As used herein, fetal restricted antigens refers to antigen that are present in pregnant women uniquely, or in substantially elevated amounts compared to non-pregnant women in maternal serum, plasma, urine, saliva, sweat, tears and  
10       other bodily fluids.

          As used herein, fetal fibronectin is a fetal restricted antigen found in placenta, amniotic fluid and fetal connective tissue. It differs structurally from adult fibronectins. Fetal fibronectin is not present in significant quantities in maternal plasma or serum. Fetal fibronectin may be captured with a general  
15       binding antibody, such as an anti-fibronectin antibody, or an anti-fetal restricted antigen antibody, such as anti-fetal fibronectin antibody.

          As used herein, an immunoassay is defined as any method using a preferential binding of an antigen with a second material, a binding partner, usually an antibody or another substance having an antigen binding site, which  
20       binds preferentially with an epitope of the fetal restricted antigen. Preferential binding, as used herein, refers to binding between binding partners that is selective and generally specific, and demonstrates less than 10%, preferably less than 5%, cross-reactive nonspecific binding. The immunoassay methods provided herein include any known to those of skill in the art, including, but not  
25       limited to, sandwich, competition, agglutination or precipitation, for example.

          As used herein, a solid support refers to the material to which the antibody is linked. A variety of materials can be used as the solid support. The support materials include any material that can act as a support for attachment of the molecules of interest. Such materials are known to those of skill in this  
30       art. These materials include, but are not limited to, organic or inorganic polymers, natural and synthetic polymers, including, but not limited to, agarose, cellulose, nitrocellulose, cellulose acetate, other cellulose derivatives, dextran,

-13-

dextran-derivatives and dextran co-polymers, other polysaccharides, glass, silica gels, gelatin, polyvinyl pyrrolidone, rayon, nylon, polyethylene, polypropylene, polybutylene, polycarbonate, polyesters, polyamides, vinyl polymers, polyvinylalcohols, polystyrene and polystyrene copolymers, polystyrene cross-  
5 linked with divinylbenzene or the like, acrylic resins, acrylates and acrylic acids, acrylamides, polyacrylamides, polyacrylamide blends, co-polymers of vinyl and acrylamide, methacrylates, methacrylate derivatives and co-polymers, other polymers and co-polymers with various functional groups, latex, butyl rubber and other synthetic rubbers, silicon, glass, paper, natural sponges, insoluble  
10 protein, surfactants, red blood cells, metals, metalloids, magnetic materials, or other commercially available media.

As used herein, a reader refers to an instrument for detecting and/or quantitating data, such as on test strips. The data may be visible to the naked eye, but does not need to be visible.

15 As used herein, a reflectance reader refers to an instrument adapted to read a test strip using reflected light, including fluorescence, or electromagnetic radiation of any wavelength. Reflectance can be detected using a photodetector or other detector, such as charge coupled diodes (CCD). A preferred reflectance reader, which is provided and described herein, includes a  
20 cassette slot adapted to receive a test-strip, light-emitting diodes, optical fibers, a sensing head, including means for positioning the sensing head along the test strip, a control circuit to read the photodetector output and control the on and off operation of the light-emitting diodes, a memory circuit for storing raw and/or processed data, and a photodetector, such as a silicon photodiode  
25 detector.

As used herein, a sensing head refers to the assembly which is adapted to read a test strip using reflected light or other electromagnetic radiation. Thus, the sensing head in the reader provided herein refers to the part of the sensing head assembly that randomizes the optical bundles and arranges the  
30 fibers in the plane normal to the test strip.

-14-

As used herein, color refers to the relative energy distribution of electromagnetic radiation within the visible spectrum. Color can be assessed visually or by using equipment, such as a photosensitive detector.

As used herein, a color change refers to a change in intensity or hue of color or may be the appearance of color where no color existed or the disappearance of color.

As used herein, a decision-support system, also referred to as a "data mining system" or a "knowledge discovery in data system", is any system, typically a computer-based system, that can be trained on data to classify the input data and then subsequently used with new input data to make decisions based on the training data. These systems include, but are not limited, expert systems, fuzzy logic, non-linear regression analysis, multivariate analysis, decision tree classifiers, Bayesian belief networks and, as exemplified herein, neural networks.

As used herein, an adaptive machine learning process refers to any system whereby data are used to generate a predictive solution. Such processes include those effected by expert systems, neural networks, and fuzzy logic.

As used herein, an expert system is a computer-based problem solving and decision-support system based on knowledge of its task and logical rules or procedures for using the knowledge. The knowledge and the logic are entered into the computer from the experience of human specialists in the area of expertise.

As used herein, a neural network, or neural net, is a parallel computational model comprised of densely interconnected adaptive processing elements. In the neural network, the processing elements are configured into an input layer, an output layer and at least one hidden layer. Suitable neural networks are known to those of skill in this art (see, e.g., U.S. Patents 5,251,626; 5,473,537; and 5,331,550, Baxt (1991) "Use of an Artificial Neural Network for the Diagnosis of Myocardial Infarction," Annals of Internal Medicine 115:843; Baxt (1992) "Improving the Accuracy of an Artificial Neural Network Using Multiple Differently Trained Networks," Neural Computation 4:772; Baxt



-15-

(1992) "Analysis of the clinical variables that drive decision in an artificial neural network trained to identify the presence of myocardial infarction," Annals of Emergency Medicine 21:1439; and Baxt (1994) "Complexity, chaos and human physiology: the justification for non-linear neural computational analysis,"

5 Cancer Letters 77:85).

As used herein, a processing element, which may also be known as a perceptron or an artificial neuron, is a computational unit which maps input data from a plurality of inputs into a single binary output in accordance with a transfer function. Each processing element has an input weight corresponding  
10 to each input which is multiplied with the signal received at that input to produce a weighted input value. The processing element sums the weighted inputs values of each of the inputs to generate a weighted sum which is then compared to the threshold defined by the transfer function.

As used herein, a transfer function, also known as a threshold function  
15 or an activation function, is a mathematical function which creates a curve defining two distinct categories. Transfer functions may be linear, but, as used in neural networks, are more typically non-linear, including quadratic, polynomial, or sigmoid functions.

As used herein, an image is a multi-dimensional array of data points,  
20 where each data point is represented by a number, or a set of numbers, and where there is a relationship between adjacent points in each of the dimensions. The index values in each dimension typically represent a linear relationship, like position or time, but are not limited to these types of relationships. A single digitized scan line from a TV frame would be considered a two dimensional  
25 image. In the case of the preferred embodiment, an image refers to a one-dimensional set of pixels, which encode the intensity of the color on the test strip.

As used herein, classifying an image refers to associating an object or state with the image. Images of fruit might be classified as to the type of fruit  
30 shown in the image. In the case of the preferred embodiment, classifying the test strip image refers to associating the positive or negative state with the image.

-16-

As used herein, reconstructing an image refers to producing an image from a mathematical function. When an image is represented by a mathematical function, there may be errors in the representation due to any number of factors.

5           As used herein, backpropagation, also known as backprop, is a training method for neural networks for correcting errors between the target output and the actual output. The error signal is fed back through the processing layer of the neural network, causing changes in the weights of the processing elements to bring the actual output closer to the target output.

10           As used herein, Quickprop is a backpropagation method that was proposed, developed and reported by Fahlman ("Fast Learning Variations on Back-Propagation: An Empirical Study", Proceedings on the 1988 Connectionist Models Summer School, Pittsburgh, 1988, D. Touretzky, et al., eds., pp.38-51, Morgan Kaufmann, San Mateo, CA; and, with LeBriere, "The Cascade-  
15   Correlation Learning Architecture", Advances in Neural Information Processing Systems 2, (Denver, 1989), D. Touretzky, ed., pp. 524-32. Morgan Kaufmann, San Mateo, CA).

As used herein, diagnosis refers to a predictive process in which the presence, absence, severity or course of treatment of a disease, disorder or  
20   other medical condition is assessed. For purposes herein, diagnosis will also include predictive processes for determining the outcome resulting from a treatment.

As used herein, risk refers to a predictive process in which the probability of a particular outcome is assessed.

25           As used herein, a patient or subject includes any mammals for whom diagnosis is contemplated. Humans are the preferred subjects.

As used herein, biochemical test data refers to data from any analytical methods, which include, but are not limited to: immunoassays, bioassays, including nucleic acid and protein based assays, chromatography, data from  
30   monitors, and imagers; measurements and also includes data related to vital signs and body function, such as pulse rate, temperature, blood pressure, data generated by, for example, EKG, ECG and EEG, biorhythm monitors and other

-17-

such information. The analysis can assess for example, chemical analytes, serum markers, antibodies, protein, nucleic acids and other such material obtained from the patient through a sample. Immunoassays are exemplified herein, but such exemplification is not intended to limit the intended scope of the disclosure, which is applicable to any test strip and test data read by an instrument, particularly a reflectance reader.

As used herein, patient historical data refers to data obtained from a patient, such as by questionnaire format, but typically does not include biochemical test data as used herein, except to the extent such data is historical, a desired solution is one that generates a number or result whereby a diagnosis of a disorder can be generated.

As used herein, a run is defined as a group of tests that include a at least one of a positive reference, positive control, negative control and any number of clinical samples within a 24 hr. period.

As used herein, symbology refers to a code, such as a bar code, that is engraved or imprinted on the test device. The symbology is any code known or designed by the user. The symbols are associated with information stored in a remote computer or memory or other such device or means. For example, each test device can be uniquely identified with an encoded symbology. It is contemplated herein that identifying and other information can be encoded in the bar code, which can be read by the reader when the test strip is read. Alternatively, the bar code or other symbology may be read by any of reading device known to those of skill in the art.

As used herein, a bar code is a symbology, typically a field of alternating dark bars and reflective spaces of varying widths, that is affixed onto or associated with an item and provides identifying information about the item. Bar codes can placed on a reflective background, and the contrast between the dark bars and reflective spaces, or the reflectivity ratio, allows an optical sensor in a reader to discern the transitions between the bars and spaces in the symbol. Bar codes are electro-optically scanned, typically using a laser or LED, and generate a signal that is transmitted to an associated computer whose memory has digitally stored therein identifying information associated with the

-18-

item. The item is thereby automatically identified by its bar code and can be tracked, or additional information can be added to the stored information associated with the encoded item.

Several bar code formats are available and are used for different purposes and can be adapted for use in the systems herein or new ones, which can be one or two dimensional or more, devised. For example, a number of different bar code symbologies exist, these symbologies include UPC/EAN codes, Code 39, Code 128, Codeabar, Interleaved 2 of 5 and many others; two-dimensional codes, such as PDF 417, Code 49, Code 16K; matrix codes (Data Code, Code 1, Vericod); graphic codes; and any others known to those of skill in the art. Preferred herein are one-dimensional codes, such as the well known Code 39 and Code 128, although two-dimensional codes (see, e.g., U.S. Patent Nos. 5,243,655 and 5,304,786, are also suitable for use herein.

The 39 bar code provides a fully alphanumeric bar code for data entry systems. This bar code is especially effective in applications that use alphanumeric data for item identification. The structure of 39 permits it to be printed by a wide variety of techniques, including offset, letterpress, fully-formed impact printers, dot matrix printers, and on-impact printing devices. Code 39 is the most widely used alphanumeric bar code. It has been accepted as a standard code by many companies and industries. Specification ANSI Draft MH10.X-1981, entitled, "Specifications for Bar Code Symbols on Transport Packages & Unit Loads," describes three different bar code symbologies. Code 39 is called 3-of-9 code in the ANSI specification. Moreover, the Depae MIL-STD-1189, dated Jan. 4, 1982, defines 39 (called 3 of 9 code) as the standard symbology for marking unit packs, outer containers, and selected documents.

Code 39 includes 9 bits, at least three of which are always 1. Code 39 can be used to encode a set of 43 characters, including upper case alphabetic and numeric (0-9) characters, as well as seven special characters (-, ., , \*, \$, /, + and %). The beginning and end characters are always an asterisk (\*). The code uses narrow and wide bars along with narrow and wide spaces, and the encoding for a single character is made up of a pattern of bars and spaces. The

-19-

code structure is three wide elements out of a total of nine elements, where an element is the area occupied by a bar or space). The nine elements include five bars and four spaces.

In Code 128, every character is constructed of eleven bars and spaces, and all 128 ASCII characters, i.e., numeric characters, upper and lower case characters, punctuation and control codes are encoded. There are three different character sets to select from: one set encodes all upper case characters and all ASCII control characters; another encodes all upper and lower case characters; and the third encodes all numeric characters. Through the use of special characters, it is possible to switch between character sets within a single code symbol. Code 128 uses four different bar and space widths. Each data character encoded in a Code 128 symbol is made up of 11 black or white modules. Three bars and three spaces are formed out of the 11 modules. There are 106 different three bar/three space combinations. Bars and spaces can vary between one and four modules wide. The stop character is made up of 13 modules. The symbol includes a quiet zone (10 x-dimensions), a start character, the encoded data, a check character, the stop character and a trailing quiet zone (10 x-dimensions) (see, e.g., U.S. Patent No. 5,262,625).

Systems for generating and reading bar codes are readily available and are well known in the art.

#### **Point of Care Diagnostic and Risk Assessment Systems**

Provided herein are systems for use at the point of care for diagnosing and assessing certain medical risks. The systems are designed for use on site at the point of care, where patients are examined and tested, and for operation remote from the site.

The systems are designed to accept input in the form of patient data, including, but not limited to biochemical test data, physical test data, historical data and other such data, and to process and output information, preferably data relating to a medical diagnosis or a disease risk indicator. The patient data may be contained within the system, such as medical records or history, or may be input as a signal or image from a medical test or procedure, for example, immunoassay test data, blood pressure reading, ultrasound, X-ray or MRI, or

-20-

introduced in any other form. Specific test data can be digitized, processed and input into the medical diagnosis expert system, where it may be integrated with other patient information. The output from the system is a disease risk index or medical diagnosis.

- 5 In a preferred embodiment, the system includes a reader, such as a reflectance or transmission reader, preferably a reflectance reader, for reading patient data, a test device designed to be read in the reader, and software for analysis of the data. In an exemplified embodiment of the system, the reader is the reflectance reader provided herein. A test strip device in a plastic housing  
10 designed for use with the reader, optionally including a symbology, such as an alphanumeric character bar code or other machine-readable code, and software designed for analysis of the data generated from the test strip are also provided.

- The system is described with reference to an exemplary test for fFN, but it is to be understood that this embodiment is exemplary, and that the system,  
15 particularly the system with the reader head, can be adapted for any suitable assay.

#### Assays

- Any assay is intended for use in the systems and methods herein. Such assays include, but are not limited to: nucleic acid detection, including using  
20 amplification and non-amplification protocols, any assay that relies on colorimetric or spectrometric detection, including fluorometric, luminescent detection, such as creatine, hemoglobin, lipids, ionic assays, blood chemistry. Any test that produces a signal, or from which a signal can be generated, that can be detected by a detector, such as a photodetector or a gamma counter, is  
25 intended for use as part of the systems provided herein. Any wavelength is intended to be included.

- Immunoassays, including competitive and non-competitive immunoassays, are among those preferred for determination of the presence or amount of analyte in a patient sample, and are exemplified herein. It is understood that  
30 immunoassays are provided for exemplification, and that the methods and systems provided herein have broad applicability to patient test data and other test data.

-21-

A number of different types of immunoassays using a variety of protocols and labels are well known. Immunoassays may be homogeneous, i.e. performed in a single phase, or heterogeneous, where antigen or antibody is linked to an insoluble solid support upon which the assay is performed.

- 5 Sandwich or competitive assays may be performed. The reaction steps may be performed simultaneously or sequentially. Threshold assays may be performed, where a predetermined amount of analyte is removed from the sample using a capture reagent before the assay is performed, and only analyte levels of above the specified concentration are detected. Assay formats include, but are not
- 10 limited to, for example, assays performed in test tubes, wells or on immuno-chromatographic test strips, as well as dipstick, lateral flow or migratory format immunoassays.

- Any known immunoassay procedure, particularly those that can be adapted for use in combination with lateral flow devices as described herein,
- 15 can be used in the systems and methods provided herein.

#### Test Device

- Any device that is compatible for use with a reader, preferably a reflectance reader, for determining the assay result is contemplated for use herein. Exemplary devices include test strips, such as lateral flow devices,
- 20 preferably contained within a housing adapted for use with the reader.

- Any such test strips that can be adapted for use in combination with a reader are contemplated for use in the systems provided herein. Such test strip devices as are known to those of skill in the art (see, e.g., U.S. Patent Nos. 5,658,801, 5,656,502, 5,591,645, 5,500,375, 5,252,459, 5,132,097 and
- 25 many other examples) may be used in systems as described herein, particularly in combination with the reader provided herein.

- Typically these test devices are intended for use with biological samples, such as, for example, but not limited to, saliva, blood, serum, cerebral spinal fluid, cervico-vaginal samples. Other biological samples, such as food samples,
- 30 which are tested for contamination, such as by bacteria or insects, are also contemplated.

-22-

Target analytes include, but are not limited to: nucleic acids, proteins, peptides, such as human immunodeficiency virus (HIV) antigens, antigens indicative of bacterial, such as Salmonella and E. coli, yeast or parasitic infections, apolipoprotein(a) and lipoprotein(a), environmental antigens, human chorionic gonadotropin (hCG), E-3-G, interleukins and other cytokines and immunomodulatory proteins, such as IL-6 and interferon, small nuclear ribonuclear particles (snRNP) antigens, fFN and other indicators, such as IGF binding protein-1, of pregnancy related disorders. Immunoassay and other tests for such antigens are known (see, *e.g.*, U.S. Patent Nos. 4,919,889, 5,079,171, 5,096,830, 5,185,270, 5,223,440, 5,236,846, 5,281,522, 5,096,830 and 5,079,171; see, also International PCT application No. WO 93/09438 and U.S. Patent No. 5,516,702; International PCT application No. WO 92/12426 and U.S. Patent No. 5,554,504; and see also International PCT application No. WO 94/17405 or EP A O 680 607, and other such tests known to those of skill in the art.

#### **Immunoassay Test Strip**

Any suitable test strip or medium for performing an assay is contemplated herein as long as the "strip" can be adapted for use with a reader as described herein. A preferred embodiment is an immunoassay test strip that includes a membrane system that defines a liquid flow pathway.

For performing immunoassays, lateral flow test immunoassay devices are among those preferred herein. In such devices, a membrane system forms a single fluid flow pathway along the test strip. The membrane system includes components that act as a solid support for immunoreactions. For example, porous or bibulous or absorbent materials may be placed on a strip such that they partially overlap, or a single material can be used, in order to conduct liquid along the strip. The membrane materials may be supported on a backing, such as a plastic backing. In a preferred embodiment, the test strip includes a glass fiber pad, a nitrocellulose strip and an absorbent cellulose paper strip supported on a plastic backing.

Antibodies that react with the target analyte and/or a detectable label system are immobilized on the solid support. The antibodies may be bound to



-23-

the test strip by adsorption, ionic binding, van der Waals adsorption, electrostatic binding, or by covalent binding, by using a coupling agent, such as glutaraldehyde. For example, the antibodies may be applied to the conjugate pad and nitrocellulose strip using standard dispensing methods, such as a  
5 syringe pump, air brush, ceramic piston pump or drop-on-demand dispenser. In a preferred embodiment, a volumetric ceramic piston pump dispenser is used to stripe antibodies that bind the analyte of interest, including a labeled antibody conjugate, onto a glass fiber conjugate pad and a nitrocellulose strip.

The test strip may or may not be otherwise treated, for example, with  
10 sugar, a polymer such as polyvinylpyrrolidone or other release agent to facilitate mobility along the test strip, or with water-soluble non-immune animal proteins, such as albumins, including bovine (BSA), other animal proteins, water-soluble polyamino acids, or casein to block non-specific binding sites.

An exemplary immunoassay test strip provided herein is shown in FIG. 1.  
15 The test strip is described in detail in EXAMPLE 1. This test strip is provided for purposes of exemplification of the methods and systems provided herein and is not intended to limit the application to immunoassay test strip devices nor to the exemplified device.

#### **Test Strip Housing**

20 The test strip or other such medium optionally may be contained within a housing suitable for reading, such as for insertion into a reader, such as the reflectance reader provided herein. The housing may be fabricated from any suitable material, including plastic or other inert material that does not interfere with the assay procedure. An exemplary assay device, including a test strip  
25 and housing assembly, is shown in FIGs. 2-5.

If desired for tracking and identification, the test strip housing or other portion thereof can include an identifying or identifiable symbology, such as a bar code. The bar code can contain information that can be associated with data related to the assay device, patient data, test run, lot numbers, calibration  
30 information, and any information.

-24-

For example, information associated with the device, such as lot number, expiration date, analyte and intensity value, or information related to the test run, such as date, reflectance value or other such information, can be encoded and associated, such as in a database with a bar code imprinted on the device.

- 5 Any bar code system that provides the appropriate line thickness and spacing can be used. Code 39 and Code 128 are among the bar code systems suitable for use in the systems herein. Other one dimensional or multidimensional (i.e., two or three dimensional coding systems can be used or developed).

- 10 In an exemplary embodiment, Code 39 is used, and one exemplary bar code is depicted in FIG. 25. The bar code contains 11 alphanumeric characters, including 2 alphabetic and 9 numeric characters. The first and last characters are asterisks (\*), as is standard in the Code 39 system. The lot number is stored as 1 alpha and 4 numeric codes so that product complaints or questions can be traced to a particular lot number. In the exemplified embodiment, the
- 15 first character represents the month of production, the second is a digit representing the year of production and the last three are an index value indicating the lot number. Thus, the lot number "A8001" represents the first device in a lot produced in January, 1998. The next two characters ("01") represent the identity of the analyte as 2 numerics (00-99). This permits the
- 20 use of up to 100 different analytes with the system. A reflectance intensity value (00-99), which sets the reference threshold for which controls and patient samples can be compared, is stored as the next two numeric characters ("01"). This eliminates the need to run liquid reference samples on a daily basis. FIGs. 2 and 3 depict assay devices that optionally include bar codes, 216 and 316,
- 25 respectively. In the exemplified embodiment, the cassette expiration date is stored as 1 alpha and 1 numeric code to prevent the use of expired devices. In the example given, an expiration code of "A9" represents an expiration date of January, 1999. Other codes can be readily employed and other information, as desired, encoded thereon.

### Antibodies

Any antibodies, including polyclonal or monoclonal antibodies, including animal, such as rodent, humanized, or any fragment thereof, such as Fab fragments, that bind the analyte of interest, are contemplated for use herein.

- 5 Monoclonal and/or polyclonal antibodies may be used. The antibody is selected for the particular target antigen.

For example, for the exemplified assay, anti-fetal fibronectin antibodies are employed. A mouse monoclonal anti-fetal fibronectin antibody has been used in a labeled antibody-conjugate for detecting fetal fibronectin, and a  
10 polyclonal goat anti-mouse antibody used to bind fetal fibronectin to form a sandwich complex. In the exemplary embodiment, an antibody that binds to the labeled antibody conjugate that is not complexed with fetal fibronectin is immobilized on the test strip and used as a control antibody. Such antibodies are known to those of skill in the art (see, *e.g.*, U.S. Patent Nos. 5,281,522;  
15 4,894,326 and 5,243,029,) and are discussed below.

### Conjugation of the Antibody to a Label

An antibody conjugate containing a detectable label may be used to bind the analyte of interest. The detectable label used in the antibody conjugate may be any physical or chemical label, such as fluorescent, chemiluminescent,  
20 bioluminescent, radio-, and enzyme labels, capable of being detected, directly or indirectly, on a solid support using a reader, preferably a reflectance reader, and capable of being used to distinguish the reagents to be detected from other compounds and materials in the assay. Suitable antibody labels are well known to those of skill in the art. The labels include, but are not limited to enzyme-  
25 substrate combinations that produce color upon reaction, colored particles, such as latex particles, colloidal metal or metal or carbon sol labels, fluorescent labels, and liposome or polymer sacs, which are detected due to accumulation of the label. A preferred label is a colored latex particle, which are well known and commercially available. In an alternative embodiment, colloidal gold is used  
30 in the labeled antibody conjugate.

-26-

The label may be derivatized for linking antibodies, such as by attaching functional groups, such as carboxyl groups to the surface of a particle to permit covalent attachment of antibodies. Antibodies may be conjugated to the label using well known coupling methods. Coupling agents such as glutaraldehyde or carbodiimide may be used. The labels may be bonded or coupled to the antibodies by chemical or physical bonding. In a preferred embodiment, a carbodiimide coupling reagent, 1-ethyl-3-(3-dimethylaminopropyl)carbodiimide (EDAC), is used to link antibodies to latex particles. Coupling reagents are well-known to those of skill in this art, and any such agent may be used. Latex particles are commercially available and also well known (see, *e.g.*, U.S. Patent Nos. 4,373,932, 4,436,826 and 4,716,123).

#### Measurement of Analytes

Any analyte that can be detected in any assay, particularly colorimetric assays, including immunoassays, and that can be associated with a disorder is contemplated for as a target herein. Suitable analytes are any which can be used, along with a specific binding partner, such as an antibody, or a competitor, such as an analog, in an assay. Analytes may include, but are not limited to proteins, haptens, immunoglobulins, enzymes, hormones (*e.g.*, hCG, LH, E-3-G estrone-3-glucuronide and P-3-G (progesterone-3-glucuronide)), polynucleotides, steroids, lipoproteins, drugs, bacterial or viral antigens, such as *Streptococcus*, *Neisseria* and *Chlamydia*, lymphokines, cytokines, and the like. A number of suitable analytes are described in U.S. Patent No. 5,686,315, which is incorporated herein by reference. Although examples are provided for the determination of fetal fibronectin in cervicovaginal samples, the systems and methods provided herein are not limited to the detection and measurement of fetal fibronectin, but apply to any biochemical test, particularly those for which test strips can be developed or for which test strips are known.

#### Measurement of Fetal Fibronectin

In an exemplary embodiment, the system is used for diagnosing or predicting conditions such as pregnancy, including ectopic pregnancy, pre-eclampsia, preterm labor or imminent delivery, fetal membrane rupture or infections of concern during pregnancy that may compromise the pregnancy or

**-27-**

harm the newborn, including, for example, ascending genital infections such as chlamydia or herpes simplex virus. Fetal fibronectin is a fetal restricted antigen found in placenta, amniotic fluid and fetal connective tissue. Since fetal fibronectin is strictly associated with pregnancy, determination of the presence of fetal fibronectin in a cervicovaginal sample is a highly reliable early indication of pregnancy. Also, the absence of a fetal restricted antigen in a cervicovaginal sample during the first 20 weeks of pregnancy is an indicator of ectopic pregnancy. Ectopic pregnancies, which are a major cause of mortality and mortality for women, are not readily distinguished from normal pregnancies using standard pregnancy determination methods and tests. Determination of impending preterm births is critical for increasing neonatal survival of preterm infants. The presence of fetal fibronectin (fFN) in cervicovaginal secretion samples in patients after week 12 of pregnancy has been shown to be associated with a risk of impending delivery, including spontaneous abortions (12-20 weeks), preterm delivery (20-37 weeks), term (37-40 weeks) and post-date delivery (after 40 weeks), in pregnant women. In addition, the presence of fetal fibronectin in a cervicovaginal sample provides a method for determining increased risk of labor and fetal membrane rupture after week 20 of pregnancy. Detection of rupture of the amniotic membrane is important in distinguishing true and false labor, and when the rupture is small and the volume of amniotic liquid escaping is small, the rupture is often undetected. The methods and systems herein provide a means to reliably assess the risk for any of these conditions. An immunoassay procedure for detecting fetal fibronectin is described in EXAMPLE 2.

## 25 Test Strip for Measuring fFN and Cellular Fibronectin

Methods for measuring fetal fibronectin and cellular fibronectin levels in cervicovaginal samples are known (see, U.S. Patent Nos. 4,919,889, 5,079,171, 5,096,830, 5,185,270, 5,223,440, 5,236,846, 5,281,522, and 5,468,619), and diagnostic tests for various pregnancy-related disorders are available (see, e.g., U.S. Patent Nos. 5,096,830 and 5,079,171) in which levels of estriol in saliva are correlated with risks of preterm delivery; International PCT application No. WO 93/09438 and U.S. Patent No. 5,516,702, which describes

-28-

the use of cytokines as indicators of risk of preterm delivery and of membrane rupture). Other tests that can be incorporated into systems provided herein include tests in which the level of insulin-like growth factor binding protein 1 (IGFBP-1) in a vaginal secretion sample, resulting from the rupture of fetal  
5 membranes, is used to detect rupture of fetal membranes (see, International PCT application No. WO 92/12426 and U.S. Patent No. 5,554,504; and see also International PCT application No. WO 94/17405 or EP A 0 680 607, which describes the use the levels IGFBP-1 in cervicovaginal samples from women determined to be at risk of preterm delivery as a means for determining the risk  
10 of impending preterm delivery). These methods can be adapted for use with the immunoassay test strips and devices described herein. In particular, an immunoassay test strip for measuring fFN in cervicovaginal samples is provided.

#### **Antibodies for Fetal Fibronectin**

An antibody that will bind the analyte of interest is conjugated to a  
15 detectable label. The selected antibody will depend upon the particular test used. Such antibodies are readily available.

In an exemplary embodiment, where fetal fibronectin is to be detected, a mouse monoclonal anti-fFN antibody (deposited at the American Type Culture Collection as accession number ATCC HB 9018; see U.S. Patent No.  
20 4,894,326; see, also U.S. Patent Nos. 5,281,522 and 5,243,029), conjugated to latex particles containing a blue dye may be used. In another embodiment, embodiment, a goat polyclonal antibody to human fibronectin is conjugated to a colloidal gold label.

In the embodiment, an antibody that binds the labeled antibody  
25 conjugate that is not complexed with fetal fibronectin is used as a control antibody. For example, where the labeled conjugate includes a monoclonal anti-fetal fibronectin antibody, a polyclonal goat anti-mouse IgG antibody is used.

The antibodies may be raised and purified using methods known to those of skill in the art or obtained from publicly available sources. For example,  
30 monoclonal antibody FDC-6 (deposited at the American Type Culture Collection as accession number ATCC HB 9018; see U.S. Patent No. 4,894,326; see, also, Matsuura et al. (1985) Proc. Natl. Acad. Sci. U.S.A. 82:6517-6521; see,

also, U.S. Patent Nos. 4,919,889, 5,096,830, 5,185,270, 5,223,440, 5,236,846, 5,281,522, 5,468,619 and 5,516,702), which is raised against whole molecule onco-fetal fibronectin from a tumor cell line, may be used.

#### **Fetal Fibronectin Assay Procedure**

5           The fetal fibronectin assay is provided as exemplary of assays and design thereof for use in the systems provided herein.

          In conducting the assay, a cervicovaginal patient sample is obtained. The sample may include fluid and particulate solids, and, thus, can be filtered prior to application to the assay test strip. The sample may be removed from the  
10   patient using a swab having a fibrous tip, an aspirator, suction or lavage device, syringe, or any other known method of removing a bodily sample, including passive methods for collecting urine or saliva. In particular, the sample may be extracted into a buffer solution, and optionally heated, for example, at 37°C and filtered. In the embodiment, where fetal fibronectin is to be detected in a  
15   sample, the sample is obtained from in the vicinity of the posterior fornix, the ectocervix or external cervical os using a swab having a dacron or other fibrous tip.

          A volume of the test sample is then delivered to the test strip (FIG. 1) using any known means for transporting a biological sample, for example, a  
20   standard plastic pipet. Any analyte in the sample binds to the labeled antibody and the resulting complex migrates along the test strip. Alternatively, the sample may be pre-mixed with the labeled conjugate prior to applying the mixture to the test strip. When the labeled antibody-analyte complex encounters a detection zone of the test strip, the immobilized antibody therein  
25   binds the complex to form a sandwich complex, thereby forming a colored stripe.

          Any unbound latex-conjugated antibody continues to migrate into a control zone where it is captured by a second immobilized antibody or other agent capable of binding the conjugate, and thereby forms a second colored  
30   stripe due to the accumulation of the dye-containing latex beads.

          The results of the assay are assessed using the reader and software

-30-

provided herein. The rapid test herein provides, at the very least, the same clinically relevant information as a fFN ELISA (an enzyme linked immunosorbent sandwich assay (ELISA) see, e.g., U.S. Patent No. 5,281,522 ) test heretofore available, but in significantly less time and at the point of care. This rapid fFN

5 immunoassay allows the user to test a cervicovaginal swab sample in about 20 minutes. When comparing the 20 minute rapid fFN test to the data from the fFN ELISA, a Kappa coefficient of 0.68 was found with a 95% confidence interval [0.62, 0.76] and an overall concordance of at least about 91.6%. These data were obtained using a system including an immunoassay test strip

10 in combination with a reflectance reader and data processing software employing data reduction and curve fitting algorithms or neural networks, as described herein. Thus, the systems herein provide results that are at the very least comparable to the ELISA, but generally are superior and more informative.

#### Reader

15 Reflectance readers and other readers, including densitometers and transmittance readers, are known to those of skill in the art (see, e.g., U.S. Patent Nos. 5,598,007, 5,132,097, 5,094,955, 4,267,261, 5,118,183, 5,661,563, 4,647,544, 4,197,088, 4,666,309, 5,457,313, 3,905,767, 5,198,369, 4,400,353). Any reader that upon combination with appropriate

20 software, as described herein, can be used to detect images and digitize images, such as symbologies, particularly bar codes or the lines and stripes produced on chromatographic immunoassay devices or on gels or photographic images thereof, such as the lines on DNA and RNA sequencing gels, X-rays, electrocardiograms, and other such data, is intended for use herein.

25 The reader provided herein, particularly in combination with the software provided herein, is preferred for use in the point of care diagnostic systems.

In an exemplified embodiment, a sample is applied to a diagnostic immunoassay test strip, and colored or dark bands are produced. The intensity of the color reflected by the colored label in the test region (or detection zone)

30 of the test strip is, for concentration ranges of interest, directly proportional or otherwise correlated with an amount of analyte present in the sample being tested.



-31-

The color intensity produced is read, in accordance with the present embodiment, using a reader device, for example, a reflectance reader, adapted to read the test strip. The intensity of the color reflected by the colored label in the test region (or detection zone) of the test strip is directly proportional to the amount of analyte present in the sample being tested. In other words, a darker colored line in the test region indicates a greater amount of analyte, whereas a lighter colored line in the test region indicates a smaller amount of analyte. In accordance with the present embodiment, the color intensity produced, i.e., the darkness or lightness of the colored line, is read using a reader device, for example, a reflectance reader, adapted to read the test strip. A reflectance measurement obtained by the reader device is, in accordance with the present embodiment, correlated to the presence and/or quantity of analyte present in the sample as described hereinbelow. The reader takes a plurality of readings along the strip, and obtains data that are used to generate results that are an indication of the presence and/or quantity of analyte present in the sample as described hereinbelow. The system also correlates such data with the presence of a disorder, condition or risk thereof.

Optionally, in addition to reading the test strip, the reader may be adapted to read a symbology, such as a bar code, which is present on the test strip or housing and encodes information relating to the test strip device and/or test result and/or patient, and/or reagent or other desired information. Typically the associated information is stored in a remote computer database, but can be manually stored. In other embodiments, the symbology can be imprinted when the device is used and the information encoded therein.

Referring to FIG. 6, an exemplary embodiment of the reader device 600 is shown with an immunoassay device 200, as shown in FIG. 2A, inserted into a cassette slot 602 therein. The cassette slot 602 is adapted to receive the immunoassay device 200, and a reader head assembly (not shown) supported within the reader device 600 is adapted to read the immunoassay test strip, and optionally a symbology, exemplified as a bar code, on with the immunoassay device. Such reading is performed by scanning a reader head (not shown) across the device, including a test window 214 in the immunoassay device 200

-32-

and a symbology, such as the exemplified bar code 216, if present, and in the process directing light onto the bar code and/or a test portion and a control portion of the immunoassay test strip. An amount of such light reflected back from the bar code and/or the test portion and control portion of the

5 immunoassay test strip is measured as the reader head scans across the device.

Also shown are a data entry keypad 604, including ten digit keys (also labeled with letters of the alphabet, such as is commonly the case on telephone keypads), a delete key, a space key, an escape key, a print key, enter key, and up, down, left and right arrow keys, additional characters such as , or . or /, and  
10 any others desired by the user. The data entry keypad 604 can be used by an operator of the reader device 600 to input identification information, to enter control test parameters, to initiate and terminate testing, and the like. A processing unit (not shown) housed within the reader device 600 is responsive to the keypad and performs data analysis functions, as described hereinbelow,  
15 in accordance with modifications made to a processor in the processing unit by an appropriate software subsystem.

Also shown in FIG. 6 is a liquid crystal display screen 606. The liquid crystal display screen 606 receives output data from the processing unit and displays it to an operator of the reader device 600, including displaying results  
20 of tests, error messages, instructions, troubleshooting information, and the like.

Referring next to FIG. 7, a perspective view of a lower housing 702 of one embodiment of an immunoassay reader device 600 of FIG. 6 is shown with a reader head assembly 704 located therein and the immunoassay device 200 inserted into the cassette slot 602 at a front edge of the lower housing 702.  
25 The cassette slot 602 located at the front edge of the lower housing 702 provides an aperture through which the immunoassay device 200 is inserted into and guided into the reader device 600 in order measure light reflected from an immunoassay test strip. In some embodiments of the reader, the reader is adapted to additionally read a symbology, such as a bar code, imprinted,  
30 engraved on or otherwise affixed to the test strip or device.

When the immunoassay device 200 is inserted into the cassette slot 602 of the lower housing, a reader head 706 on the reader head assembly 704 is

-33-

positioned directly above the device 200, such that the longitudinal (or major) axes of optical fibers within the reader head 706 are normal to a surface of the device, including the test strip and optionally a symbology that is imprinted, engraved or other wise affixed on the device.

5           Alternatively, the reader head 706 may be fixed, at least rotationally, and the immunoassay device 200 may be moved into position after insertion into the cassette slot 602, such that the longitudinal (or major) axes of optical fibers within the reader head 706 are normal to a surface of the device to be read by the reader.

10           Referring next to FIG. 8, a top view is shown of the lower housing 702, the immunoassay device 200, the cassette slot 602, and a stepper motor 802. As can be seen, after insertion into the lower housing 702, the immunoassay device 200 is positioned in alignment with the stepper motor 802, which is part of the reader head assembly. The stepper motor is used to scan the reader  
15 head 706 across the symbology, such as the exemplified bar code 216 and/or test window 214 of the immunoassay device 200.

One embodiment of the reader device is shown in FIG. 9. Shown are the lower housing 702, the immunoassay device 200, the stepper motor 802, an actuator wheel 902, the reader head 706, and linkages for moving the reader  
20 head 706 parallel to a major axis of the immunoassay device 200 in order to scan the reader head 706 across the symbology (bar code) 216 and/or test window 214 of the immunoassay device 200.

To read the immunoassay test strip, the reader head is brought within a uniform distance of about 0.010 inches from the test strip. When the  
25 immunoassay device 200 is slid into the cassette slot 602, the actuator wheel 902 and an actuator spring (not shown) work together to bring the reader head 706 down to within about 0.010 inches of the immunoassay test strip within the housing 202 of the immunoassay device 200. In order to move the reader head 706 into position within 0.010 inches of the immunoassay test strip, the  
30 reader head 706 is pivoted along with a portion of the reader head assembly. Prior to being brought into position within 0.010 inches of the immunoassay test strip, while the immunoassay device 200 is being inserted into or removed

-34-

from the immunoassay reader device 600, the reader head 706 assumes a retracted position, i.e., raised position, so that the immunoassay device 200 can be inserted into or removed from the immunoassay reader device 600 without crashing the reader head 706 into the immunoassay device 200.

- 5           When the immunoassay device 200 is inserted into the cassette slot 602, it contacts the actuator wheel 902 and causes a carriage assembly of the reader head assembly to be brought down from the retracted position so that the reader head 706 is within 0.010 inches of the immunoassay test strip.

- Insertion of the immunoassay device 200 causes the actuator wheel to  
10   pop-up by applying pressure to the actuator spring, bringing the carriage assembly down from the retracted position.

- The immunoassay device 200 is pushed into the cassette slot 602 until it meets a stop. Once inserted, the immunoassay device 200, the actuator wheel 902, and the actuator spring remain fixed in position, while the reader head 706  
15   is stepped across the test window 214 of the immunoassay device 200 by the stepper motor 802. In other words, only the reader head 706 moves during the scanning of the immunoassay test strip.

- Alternatively, the immunoassay device 200 is pushed into the cassette slot 602 until it meets the stop. Once inserted the immunoassay device 200  
20   may be rotated up to within 0.010 inches of the reader head 706 by gently lifting the immunoassay device 200. By gently lifting the immunoassay device 200, a base of the reader head assembly is pivoted up toward the carriage assembly and the reader head 706, positioning the immunoassay test strip within 0.010 inches of the reader head 706. Then the reader head 706 is then  
25   stepped across the test window 214 of the immunoassay test strip by the stepper motor 802. In other words, in accordance with this alternative, only the reader head 706 moves during the scanning of the immunoassay test strip and, the reader head 706 moves only during the scanning of the immunoassay test strip.

- 30           Prior to insertion of the immunoassay device 200 into the cassette slot 602, and prior to scanning, the reader head 706 is positioned at a point that would place it approximately half way across (in the middle of) the test window

-35-

214 of the immunoassay device 200. After insertion of the device 200 into the reader 600, when an operator depresses a scan key on the key pad (see FIG. 6), the reader head 706 is moved from this position toward the stepper motor 802 until a microswitch is activated. Once the microswitch is activated, the

5 reader head 706 is said to be in a "home" position from which scanning of the test strip commences. Once scanning commences, the reader head 706 advances from the home position across the test window 214. Thus, the reader head 706 scans in a direction moving away from the stepper motor toward the cassette slot 602 or to the left as depicted in FIG. 9. Total travel of

10 the reader head 706 during scanning of the immunoassay test strip is 0.452 inches, which is achieved in 0.002 inch steps, which are 226 in number. One set of readings is taken per step, with each set of readings including a dark reading, a first light reading and a second light reading.

Referring next to FIG. 10, the reader head assembly 1000 is shown.

15 Shown are the actuator spring 1002, the actuator 1004, the base 1006, the stepper motor 802, the actuator wheel 902, a rotor arm 1008, and the reader head 706. Also shown is a pivot point 1010 on which the carriage assembly 1012, including the reader head 706, stepper motor 802, actuator wheel 902, actuator spring, 1002, and rotor arm 1008 pivot to assume a raised position for

20 insertion and removal of the immunoassay device 200 from the reader device 600 and to assume a lowered position for scanning the reader head 706 across the test window 214 of the immunoassay device 200.

Referring next to FIG. 11, shown is a side view of the reader head 706 of the reader head assembly of FIG. 10. Shown is a first light emitting diode

25 (LED) 1102, a second light emitting diode (LED) 1104, a photodetector 1106, a reader head aperture 1108, and mounting holes 1110.

Referring next to FIG. 12 a reverse angle side view is shown of the reader head assembly 1000 of FIG. 10. Shown are the stepper motor 802, the base 1006, mounting holes 1202, and a mounting bracket 1204 on which the

30 reader head 706 is mounted.

-36-

Referring next to FIG. 13 a reverse angle side view of the reader head 706 of FIG. 11 is shown. Seen are the mounting holes 1110, and the reader head aperture 1108.

Referring next to FIG. 14, shown is a side view of the reader head assembly 1000 of FIG. 10 having assumed a retracted position. Shown are the actuator spring 1002, the actuator arm 1004, the stepper motor 802, the reader head 706, the reader head supporting bracket 1204, the pivot 1010 on which such elements rotate, and a base 1006 relative to which such elements rotate.

As can be seen, the actuator arm 1004, the actuator spring 1002, the stepper motor 802, the reader head 706, the reader head mounting bracket 1204, and mechanisms used for supporting and scanning the reader head 706 are designed so that the test strip 214 in the device 200 is positioned within 0.010 inches of the aperture 1108 of the reader head. Any design suitable to effect such can be employed with the present embodiment.

In the example illustrated, the actuator arm 1004, the actuator spring 1002, the stepper motor 802, the reader head 706, the reader head mounting bracket 1204, and the mechanisms used for supporting and scanning the reader head 706 are shown rotated on the pivot 1010 such as would be the case, in accordance with the variation shown, when the immunoassay device 200 has been removed from the reader device 600 and/or as the immunoassay device 200 is being inserted into or removed from the reader device 600.

Referring next to FIG. 15, a side view is shown of the reader head 706 of FIG. 11. Shown are the aperture 1108 and the first light emitting diode 1102.

Referring next to FIG. 16, an end view is shown of the reader head assembly 1000 of FIG. 10. Shown is the stepper motor 802, the base 1006, and the actuator arm 1004.

In alternative embodiments, the reader is adapted to read a symbology, such as a bar code. An exemplary embodiment of a reader so-adapted is shown in FIG. 24. In this embodiment, when the device cassette 2402 is inserted into the reader, it sits on a spring stage 2404. Prior to insertion of the device 300

-37-

(as shown in FIG. 2B) into the cassette slot 602, and prior to scanning, the reader head 2406 is positioned at a point that would place it approximately 0.125 inches from the forward edge of the device as it is inserted into the reader.

- 5           As shown in FIG. 2B, the device includes guide ridges 318 on either side of the bar code along the outer edges of the upper surface of the device. The reader head 2406 is moved by the shaft 2408 of the stepper motor 2414 and scans in a direction moving away from the stepper motor toward the cassette slot 2412. As the reader head 2406 moves along the device above the bar
- 10   code 2410, the guide ridges 2412 contact the reader head assembly and act to compress the spring stage 2404 by 3° in order maintain the reader head 2406 at a distance of 0.010 inches above the bar code 2410 as the bar code 2410 is read. After the bar code 2410 is read, the reader head assembly 2406 moves off the guide ridges 2412, the spring stage 2404 returns to a level position
- 15   (0°), and the reader head 2406 is repositioned at a distance of 0.010 inches in order to read the test strip. When reading a symbology, such as a bar code, the reader is moved in steps of approximately between 0.002-0.008 inches at a scan resolution of approximately 125-500 steps per inch, preferably about 250 steps per inch. One set of readings is taken per step, with each set of readings
- 20   including a dark reading, a first light reading and a second light reading.

Regardless of whether one of these alternatives is used, or whether any of numerous variations thereof or any of numerous other possible embodiments well within the abilities of the skilled artisan to easily produce is used in order to position the reader head within a prescribed distance, e.g., 0.010 inches, of the

25   test strip symbology, such as a bar code, a suitable mechanism is preferably employed to effect such positioning.

Referring next to FIG. 17, shown is a side view partially in cross-section of an exemplary embodiment of the reader head. Shown are a first light emitting diode 1102, a second light emitting diode 1104 and a photodetector

30   1106. Also shown is an aperture 1108 and the mounting holes 1110. Shown coupled between each of the LED's 1102, 1104 and the aperture 1108 are first and second fiberoptic bundles 1702, 1704. Similarly, a third fiberoptic bundle

-38-

1706 is shown coupled between the aperture 1108 and the photodetector 1106. The first and second fiberoptic bundles 1702, 1704 conduct light from the first and second LED's 1102, 1104, respectively, to the aperture 1108. The third fiberoptic bundle 1706 conducts light from the aperture 1108 to the  
5 photodetector 1106. In response to such light, the photodetector generates a reflection signal, e.g., a voltage indicative of an amount of reflected light. The electrical signal can be then processed and converted to a digital signal by using any method commonly known to those of skill in the art.

Referring next to FIG. 18, shown is a closeup partial cross-sectional view  
10 of the aperture 1108 of FIG. 17. Also shown are individual fiberoptic fibers 1802, 1804, 1806 of the fiberoptic bundles 1702, 1704, 1706 of FIG. 17, positioned within the aperture 1006 so as to transmit light 1808 from the aperture 1108 onto the symbology (exemplified bar code) and/or test strip 100 and to receive reflected light 1808 from the bar code and/or test strip 100  
15 entering the aperture 1108. (The transmitted and reflected light 1808 is represented with an arrow.) As can be seen, a gap 1810 between the aperture 1808 and the bar code and/or test strip 100 is present. The gap 1810 preferably has a width of approximately 0.010 inches, which is maintained as the reader head 706 is scanned across the bar code and/or test window 214 of  
20 the test strip 100.

Referring next to FIG. 19, a bottom view is shown of individual fiberoptic fiber ends 1902, 1904, 1906 positioned in the aperture 1108 of the reader head 706 of FIG. 10 so as to maximize the distribution of light emitted from individual fiberoptic fibers (fiberoptic conductors), and furthermore to maximize  
25 the uniformity of light received into individual fiberoptic conductors. Indicated using diagonal cross-hatching angled from lower left to upper right are individual fiberoptic conductor ends 1902 of the first fiberoptic bundle 1702. These individual fiberoptic conductor ends 1902 carry light emitted from the first light emitting diode from the first fiberoptic bundle through the aperture 1108 of the  
30 reader head 706. Similarly, indicated with cross-hatching from an upper left to lower right are fiberoptic conductor ends 1904 of the second fiberoptic bundle 1704. These individual fiberoptic conductor ends carry light emitted from the



-39-

second light emitting diode to the aperture 1108 of the reader head 706.

Without cross-hatching are shown individual fiberoptic conductor ends 1906 of the third fiberoptic bundle 1706. The third fiberoptic bundle 1706 carries light entering the aperture 1108 to the photodetector.

- 5 By employing the particularly advantageous arrangement of the fiberoptic conductor ends 1902, 1904, 1906 at the aperture 1108, uniform distribution emissions and light reception is achieved. Such arrangement is said to be a "sigmoidal" (S-like or serpentine) arrangement or a "sigmoidal" distribution. It is an important feature of the present embodiment that the fiberoptic fibers in
- 10 each of the three groups are arranged along with fiberoptic fibers from the remaining groups in a sigmoidal-like (or "S"-like) pattern with three columns of thirteen fiberoptic fibers each. An arrangement that achieves this feature is intended herein.

- In order to achieve the sigmoidal arrangement of fiberoptic conductor
- 15 ends shown, 39 fiberoptic conductors are positioned within the aperture 1108. Next, a clamp assembly made up of a "U"-shaped channel, and an "I"-shaped clamp positioned at the open side of the "U" is employed. The fiberoptic conductors, portions of which protrude from the aperture 1108 are placed between the "U"-shaped channel and the "I"-shaped clamp and a compressive
- 20 force is applied thereto by the "I"-shaped clamp, holding the protruding portions of the fiberoptic conductors firmly in position. A resin is then poured into the reader head 706 so as to become interposed between and around the fiberoptic conductors at the aperture 1108. Once the resin is set, the clamp assembly is removed, and the protruding portions of the fiberoptic conductors are trimmed
- 25 back flush with the aperture 1108, so as to define a planar surface of fiberoptic conductor ends 1902, 1904, 1906 at the aperture 1108. This planar surface is held parallel to a plane at an upper surface of the immunoassay test strip 100 during scanning of the immunoassay test strip.

- Advantageously, by creating this planar surface of fiberoptic conductor
- 30 ends 1902, 1904, 1906, the associated fiberoptic conductors of which all of which have longitudinal axes that are substantially parallel to one another and normal to the plane defined by the fiberoptic conductor ends 1902, 1904,

-40-

**1906.** As a result, very efficient transfer of light to and from the fiberoptic conductor ends **1902, 1904, 1906** is achieved.

Once the fiberoptic conductor ends **1902, 1904, 1906** are set in the resin, and trimmed, as described above, individual fiberoptic conductors are  
5 tested by projecting light individually through the fiberoptic conductors toward the fiberoptic conductor ends **1902, 1904, 1906**, to locate the fiberoptic conductor end associated with the particular fiberoptic conductor being tested. This determination is made by observing which of the fiberoptic conductor ends **1902, 1904, 1906** "lights up" when light is transmitted down the particular  
10 fiberoptic conductor. As fiberoptic conductors associated with the fiberoptic conductor ends **1902, 1904, 1906** are identified, the fiberoptic conductors are assigned to one of the first, second, and third fiberoptic bundles, so as to achieve, for example, the sigmoidal distribution of fiberoptic conductor ends **1902, 1904, 1906** illustrated in FIG. 19.

15 Advantageously, by effecting the sigmoidal distribution of fiberoptic conductor ends **1902, 1904, 1906** associated with fiberoptic conductors of each of the first, second, and third fiberoptic bundles, a uniform distribution of light emitted from the aperture **1108**, and a uniform distribution of light reflected back to the aperture **1108** is achieved.

20 Referring next to FIG. 20, a cross-sectional view of a first fiberoptic bundle **1702** is shown with individual fiberoptic elements **2002** selected to effect the sigmoidal distribution of FIG. 19. As can be seen, 13 individual fiberoptic elements are present in the fiberoptic bundle **1702**, which is the same number of fiberoptic conductor ends **1902, 1904, 1906** depicted in FIG. 19 for  
25 each of the three fiberoptic bundles **1702, 1704, 1706**. The fiberoptic bundle **1702** shown in FIG. 17 carries the light from the first light emitting diode to the aperture **1108** of the reader head **706**. Cross-sectional views of the second and third fiberoptic bundles are similar to that shown in FIG. 20.

Referring next to FIGs 21, 22 and 23, three schematic views are shown  
30 illustrating a process for reading test results from immunoassay test strip **100** with the control region **2102** and the detection region **2104** depicted thereon. In the example shown, blue latex particles are detected in the test region and

-41-

the control region on a nitrocellulose support. Also depicted are the aperture 1108 of the reader head 706 in a dark reading mode (FIG. 21), a first light reading mode (FIG. 22) and a second light reading mode (FIG. 23).

The reader head assembly (described above) includes the first light-  
5 emitting diode (which in the present example is a blue LED), the second LED (which in the present example is an amber LED), a silicon photodiode detector, and fiberoptic fibers arranged with fiberoptic conductor ends 1902, 1904, 1906 in the sigmoidal distribution in the aperture 1108 (e.g., 0.002 inches wide), which is located at the bottom (or tip) of the reader head 706 at a point nearest  
10 the immunoassay test strip, when the immunoassay device is inserted into the immunoassay reader device. It is understood that the selection of LEDs will be dependent upon the signal produced in the test; all detectable electromagnetic wavelengths, preferably visible light, are contemplated herein. Fluorescence and other such labeling means are also contemplated herein.

15 The blue LED and the amber LED emit light of specified wavelengths ( $\lambda_1$  and  $\lambda_2$ , respectively). It should be understood that any suitable wavelengths may be selected. Such selection is dependent on the particular assay with which the immunoassay reader device is being employed. The wavelengths selected are selected so as to allow removal of effects of the background of the  
20 immunoassay test strip or symbology, e.g., bar code, from the reflectance readings, and to optimize a reading of a reduction in reflectance associated with accumulated label at the reaction regions of the immunoassay test strip.

In an exemplary embodiment, where blue latex particles are detected on a nitrocellulose support, light having a wavelength of 430 nm (blue) is emitted  
25 from the first light emitting diode (LED<sub>1</sub>), i.e., the blue LED, into the first fiberoptic bundle 1702. The same wavelengths can be used to read a symbology, such as a bar code, associated with the assay device. The first fiberoptic bundle 1702 transmits blue light to the aperture 1108 in the reader head 706 where it is emitted at an orientation normal to a plane at the upper  
30 surface of the symbology (exemplified bar code) or test strip. A second light emitting diode (LED<sub>2</sub>), i.e., the amber LED, emits light with a wavelength of 595 nm (amber) into a second fiberoptic bundle 1704. The second fiberoptic bundle

-42-

1704 transmits the amber light to the aperture in the reader head 706 where it is emitted at an orientation normal to the plane at the upper surface of the bar code or test strip.

At the aperture, individual fiberoptic conductor ends 1902, 1904 of the first and second fiberoptic bundles 1702, 1704, along with individual fiberoptic conductor ends 1906 from the third fiberoptic bundle 1706 are arranged in three groups of thirteen optical fibers each: the first group from the first fiberoptic bundle 1702, which transmits light emitted by the blue LED to the aperture 1108; the second group from the second fiberoptic bundle 1704, which transmits light emitted by the amber LED to the aperture 1108; and the third group, which transmits reflected light received at the aperture 1108 through the third fiberoptic bundle 1706 to the photodetector. The thirty-nine fibers (thirteen in each of three groups) each include respective fiberoptic conductor ends 1902, 1904, 1906 arranged in the sigmoidal distribution (or pattern) (see FIG. 19) at the aperture 1108 such that the fiberoptic conductor ends 1902, 1904, 1906 are co-planar at the aperture and in the plane parallel to the plane at the upper surface of the bar code or test strip, when the reader head 706 is positioned to take measurements from the bar code or test strip 100.

At the fiberoptic conductor ends 1902, 1904, 1906, each fiberoptic fiber (or conductor) has a longitudinal axis that is normal to the plane at the upper surface of the bar code or test strip. As a result, light emitted from the fiberoptic conductor ends 1902, 1904, 1906 is directed in a direction substantially normal to this surface plane. The fiberoptic fibers in each of the three groups are arranged along with fiberoptic fibers from the remaining groups in a sigmoidal (or "S"-like) pattern with three columns of thirteen fibers each.

When the immunoassay device is inserted into the cassette slot at the front of the immunoassay reader device 600, the reader head 706 is positioned directly over the bar code or test opening of the assay device such that the longitudinal axes of the optical fibers at their ends 1902, 1904, 1906 at the aperture, are normal to a plane at the surface of the immunoassay test strip and the ends 1902, 1904, 1906 of the fibers at a distance of about 0.010 inches.

-43-

Light from the first LED and the second LED is transmitted by the fibers onto the bar code or assay test strip at an angle normal to the upper surface of the immunoassay device, and light is reflected normally back from the strip to the ends 1902, 1904, 1906. This reflected light is transmitted by the fibers of the  
5 third fiberoptic bundle to the photodetector.

The reader head 706 takes three separate reflectance readings (FIGs. 21, 22 and 23, respectively) from each position at which it reads of the immunoassay test strip. Such measurements are made by reading an output of the photodetector (which is a voltage) while controlling the first and second  
10 LED's.

The first reading is used to determine an amount of ambient (or background) light leaking into the immunoassay device (e.g., light leaking through the cassette slot entrance, or light reflected/transmitted into the reader through the housing of the immunoassay device, which may be, for example,  
15 white plastic. The first reading is a "dark" reading taken with the blue LED and the amber LED both turned off. This dark reading (which is a voltage at the photodetector) is digitized in a conventional manner using an analog to digital converter, and may be subtracted by the processing unit from other "light" readings made in response to blue LED illumination and amber LED illumination  
20 so as to correct for this light leakage.

The second reading, used to determine levels of light reflections associated with the background of the bar code or the assay test strip itself, is taken with the blue LED pulsed on and the amber LED turned off.

The third reading, used to detect the bar code or the presence of the  
25 label on the assay test strip is taken with the amber LED pulsed on and the blue LED turned off.

A control circuit (including the processing unit, which includes a processor, such as a microprocessor) receives the digitized output of the photodetector for all three readings, controls the on and off operation of the  
30 blue LED and the amber LED, controls when photodetection readings are taken, and controls the position of the reader head 706 by controlling the stepper motor. A memory circuit stores raw and/or processed data (i.e., readings from

-44-

the photodetector). The data may also be displayed to the operator via the LCD display of the immunoassay reader device 600.

After being positioned above the housing, the reader head 706 is moved (scanned) across the bar code and/or test strip by the stepper motor under the control of the control circuit to allow the reader head 706 to scan the exposed surface of the bar code and/or assay test strip (including the detection and control zones through the test window 214 in the immunoassay device). As stated above, in a preferred embodiment, the distance between reader head 706 and the bar code or assay test strip 200 is approximately 0.010". The precise distances for any system may be empirically determined and will vary between systems and even among similar systems.

The reader head 706 is slidably connected to a rail (e.g., guide rods), and is coupled to a worm or screw gear driven by the stepper motor.

Under the control of the control circuit, the stepper motor drives the reader head 706 along the rail in small steps. At each step, the control circuit takes the three readings described above ("dark", blue LED illuminated, amber LED illuminated). The control circuit moves the reader head 706 such that the fiberoptic conductor ends 1902, 1904, 1906 pass directly above and normal to the exposed surface of the bar code and/or test strip in a sequence of small steps. As explained above, during each step a sequence of "dark", blue LED and amber LED readings are taken and recorded.

The raw data read from the photodetector is then processed by the control circuit to discern the symbology, such as a bar code pattern, in order to provide information regarding the assay device and/or test run and/or reagents, and/or patient and/or to read the test strip to determine the presence or concentration of analyte in the sample.

In a preferred embodiment, when reading the test strip, since the detection and control latex stripes are each about 0.020" wide, and since each step of the sensing head is about 0.002" long, there will be about 10 steps within each stripe, i.e., within the test region and the control region. Thus, there will be 10 sets of three readings (i.e., dark, blue LED and amber LED) at the test region and 10 sets of three readings (i.e., dark, blue LED and amber

-45-

LED) at the control region. The remainder of the reading sets will not be made over either the test region or the control region.

In a preferred embodiment, when the assay device is inserted into the cassette slot of the reader device 600, the reader head 706 is positioned over the bar code or test strip, and the control circuit then moves the head to an initial (or home) position. The control circuit moves (scans) the head across the exposed surface of the bar code or test strip, including the test region and the control region of the strip, in small increments. At each step, the control circuit takes the first reading (FIG. 21) of the photodetector output with the blue LED and the amber LED, both off, takes the second reading (FIG. 22) with the blue LED pulsed on and the amber LED off, and takes a third reading (FIG. 23) with the blue LED off and the amber LED pulsed on. The control circuit then steps the reader head 706 by controlling the stepper motor and repeats the three readings at its new location. For the test strip, this process is repeated for each of 226 steps (0.452" at 0.002"/step) until the surface of the assay test strip is read. Where a bar code is read, the length of the bar code is typically approximately 1 inch in length, and a step size of approximately 0.002-0.008 inches are used; thus between approximately 125-500 steps are performed.

The raw reflectance data is then analyzed by the control circuit in accordance with appropriate software control to identify the symbology, such as a bar code or determine the presence or concentration of the analyte in the sample. Where the reader is used to read a bar code associated with the test device, the data collected from the bar code are transformed into integrated peak information and analyzed as alphanumeric characters to provide information about the assay device and/or test run. Where the reader is used to detect an analyte, the data collected from the test strip are compared to a threshold or reference reflectance value to determine the presence or concentration of the analyte. The output can be displayed via an operator interface, or can be output to another computer or apparatus.

### **30 Data Analysis and Decision Support Systems**

The systems herein include software for data analysis. Data analysis includes any algorithms or methodology for obtaining diagnostically relevant

-46-

information from the raw data. Simple algorithms as well as decision-support systems, particularly neural networks are contemplated herein.

In particular embodiments, the data analysis methodology includes, some or all of the following steps: (1) optionally correcting the reflectance readings to  
5 correct for light leakage; (2) reducing the raw reflectance data by using a ratiometric formula; (3) generating an image of the test data by plotting the reduced data; (4) expressing this image as a polynomial mathematical function, for example, by using a combination of a flat or parabolic image to represent the baseline and two gaussian curves to represent the peaks; (5) using a curve-  
10 fitting algorithm to generate parameters to define the image; (6) optimizing the reconstruction of the image and producing a fitted image; (7) comparing the scanned image and fitted image by solving the linear regression through the curves; (8) validating the parameters obtained from the curve-fitting and the peak heights obtained; and (9) classifying the validated result as positive or  
15 negative by comparing peak heights of a clinical sample to reference samples. The method may further include: (10) using the test result with other patient information in a decision-support system to generate a medical diagnosis or risk assessment.

In alternative embodiments, the parameters used to define the image, as  
20 in (5) above, and to classify the sample, as in (9) above, can be generated using trained neural networks.

#### **Data Reduction**

In an exemplary embodiment, the raw reflectance data obtained from the instrument are stored as an array of points containing a number of rows (n)  
25 corresponding to the number of points at which readings were taken along the test strip, and a number of columns (m) corresponding to the reflectance readings taken at each point, including background or dark readings and readings at different wavelengths. If necessary, the reflectance readings are processed by first subtracting the dark reading taken at the corresponding step  
30 to correct for light leakage, which typically is negligible. The corrected reflectance readings are then input into a ratiometric algorithm, which removes noise from the membrane and normalizes data between test strips:



-47-

$$f(y) = [(R_{\lambda 1}/R_{\max/\lambda 1} * R_{\max/\lambda 2}/R_{\lambda 2})].$$

The algorithm is based upon the ratio of readings at the different wavelengths and calculates a reduced data set (1 x n), which is used to generate a curve from the original reflectance data. In processing the data, a

- 5 new column of reduced data is generated by using the ratiometric formula.

When reading an assay test strip, as described above, the size of the matrix is 4 x 226, where 4 is the number of columns of data collected and 226 is the number of steps, or readings, taken along the test strip. The first column contains information about the location on the test strip from which the data are  
 10 obtained; the second column is the reflectance in the absence of illumination by the instrument (dark reading); the third column is the reflectance when the test strip is illuminated at the first wavelength (e.g. 430 nm); and the fourth column is the reflectance when the test strip is illuminated at the second wavelength (e.g. 595 nm). The information in the second column is usually zero, unless a  
 15 light breach has occurred with the instrument. The reflectance values in the third and fourth column are preferably in the 3,000-24,000 range.

Where a bar code is read, between approximately 125-500 steps are performed in reading the bar code, therefore, the matrix size would be between 4 x 125 and 4 x 500.

- 20 In the preferred embodiment described herein, the ratiometric formula would read as follows:

$$f(y) = [(R_{430nm}/R_{\max/430nm} * R_{\max/595nm}/R_{595nm})] - 1.$$

- The algorithm calculates a reflectance ratio for each step, generating a fifth column of data. The information contained in the first, third and fourth  
 25 columns can be converted into an image by plotting the first column (x-value) against the fifth column (y-value). Thus, the original data array has been converted to a 2-dimensional image, or an array of the size 1 x 226. The reflectance ratio is then plotted as a function of each step. In reading an assay test strip, as described above, the result is a two-peak graph with the peaks  
 30 occurring at the two stripes, corresponding to the detection and control zones. The reflectance data may then be further processed to obtain an accurate determination of analyte concentration in the patient sample.

-48-

Where a bar code is read, a graph is produced that corresponds to the reflectance pattern of the bar code. Pattern matching is then performed using any of a number of methods commonly known to those of skill in the art in order to identify the bar code and associate it with the particular assay run.

## 5        **Generating and Validating Images**

The image created by a plot of the data obtained from reading an assay test strip, as described above, has three basic components: a baseline or background that is either flat or parabolic; a peak corresponding to the detection zone that is gaussian; and another peak corresponding to a control zone that is  
10    also gaussian.

The parabolic component can be defined using 3 variables:

$$f(y) = Ax^2 + Bx + C.$$

Each of the gaussian curves can be defined using 3 variables:

$$f(y) = \text{Area} * [\exp^{-(x-\mu)^2/2\sigma^2}]/(\sigma(2\pi)^{1/2})$$

15        where        Area = area contained within the gaussian;  
                       $\mu$  = x-value of center position; and  
                       $\sigma$  = width.

A second plot can be generated from the three component curves, using 9 variables. This process is accomplished using a curve-fit algorithm. Such  
20    algorithms are well known to those of skill in the art, and any such algorithm may be used. Alternatively, the 9 parameters may be obtained using neural networks, as described below. From the parameters generated from the curve-fit function, a showfit function is used to generate an image from the fitted data. For example, in the preferred embodiment, a showfit function is used to  
25    generate a 1 x 226 matrix representing the fitted curve defined by the 9 parameters.

The fitted image is then compared to the original scanned image, which is produced by plotting the 1 x 226 data points as discussed above, to measure the performance of the curve-fit function. This is accomplished by plotting the  
30    fitted image against the scanned image and solving the linear regression through these values. The fitted image is then compared to the original image by plotting the fitted image against the scanned image and solving the linear

-49-

regression through the values. The fit must meet predetermined validation criteria, which are determined empirically, as discussed below. An exact match between the scanned and fitted image would yield a line with slope = 1 and r-square ( $r^2$ ) = 1.

- 5           Once the curves have been fitted, the peak height of the curve in the detection zone is determined by subtracting the parabolic baseline from the maximum peak height. The peak height is then compared to that of a previously run sample of known analyte concentration. If the peak height of the clinical sample is greater than the peak height of the reference sample, then the
- 10 test result is positive. If not, a negative test result is returned. The peak height of the curve representing the control zone may also be checked to determine if it meets a required minimum height, in order to test that the system is functioning.

- Alternatively, peak areas may be calculated and compared to give a
- 15 determination of analyte concentration in the sample. The graph may be mathematically analyzed, with a sigmoidal calculation across the background and a gaussian calculation to integrate the area beneath each of the two peaks. The analyte concentration is then determined based upon the ratio of the integrated area beneath each of the two peaks.

20           **Methods for Reducing the Image to Parameters**

- Images or large sets of data, are not readily amenable for developing and training neural net analyses. For large data sets, the number of inputs required for neural network training must be reduced. To do this assumptions regarding the types of data that can be omitted are made. As a result of the loss of
- 25 information, the performance of subsequently trained neural nets will hinge on the validity of the assumptions made. A method for reduction of data that reduces dimensionality with minimal or no loss of information will avoid this problem. The reduced database can be validated by using it to reconstruct the original dataset. With minimal or no loss of information, subsequently trained
- 30 networks should yield higher performance than networks that are trained with less complete data. Methods are provided herein for reducing dimensionality with minimal loss of information. These methods are directly applicable to the

-50-

images that are generated and data generated from the test strips described herein and is also generally applicable to all images and large datasets.

#### Methods for Optimizing the Reconstructed Image

Parameters for a mathematical function designed to reproduce, or  
5 approximate the scanned image are effective at determining the concentration of the compound being tested and thereby providing a means to classify the sample being tested. Examination of the data, for example, from the fFN test provided herein demonstrates that a scanned image can be constructed from three basic elements. There is a background density, referred to herein as the  
10 baseline density. Superimposed on the baseline are the two peaks. The first peak is referred to as the control peak and the second is the test peak. Since the shape of these peaks is very similar to a normal curve, it was assumed that the peaks have a gaussian shape. One characteristic of the "normal curve" that can be exploited is that the area under the curve is always 1.0. By modifying  
15 the formula, the height of a peak can be determined from a single function parameter.

When analyzing an image, the peak density function used is:

$$\text{Peak Density} = \text{Height} * \text{EXP}(-Z^2/Z)$$

where  $Z = (X - \text{Pos}) * S$ ,

20

$X = \text{Pixel Number}$ ,

$\text{Pos} = \text{Pixel number of center of peak}$ ,

$S = \text{Spread or width of the peak}$ , and

$\text{Height} = \text{Height of the peak}$ .

This function contains three parameters, Height, S and Pos. When the three  
25 parameters are set correctly, this function will closely match one of the peaks in the test strip image. With two peaks in the image, this function can also be used to estimate the second peak. With two peaks, there are six parameters so far that must be optimized. The goal of the optimization will be to change the above parameters in such a way as to reconstruct the image as closely as  
30 possible.

In order to reconstruct the image completely, the baseline of the image must also be estimated. Examination of scanned images showed that the

-51-

baseline had a slight curve. By using a parabolic or quadratic form function, the baseline density is estimated. The function for the base density is,

$$\text{Base Density} = X * X * \text{Curve} + X * \text{Slope} + \text{Offset}.$$

Thus, the image can be accurately reconstructed by combining these three

5 function in the following summation,

$$\text{Image Density} = \text{Base Density} + \text{Control Peak Density} + \text{Test Peak Density}.$$

This results in a total of nine parameters that must be optimized for an accurate reconstruction of the image.

10 The basic problem with attempting to fit this complex function to the test strip image is that there are no simple means for finding the optimal values for function parameters as there are for linear regression. There are many numerical techniques that can be used to optimize the parameters of the above image density function, for example, the downhill simplex method (see, "Numerical Recipes in C", Second Edition, Cambridge University Press, 1992).

15 The basic method of optimization uses an iterative approach to optimize the function parameters based on a defined cost function. Here the cost function is defined as the sum of the squares of the differences between the original image and the reconstructed image for every pixel in the scanned image. The downhill simplex method uses a simplex to accomplish this  
20 optimization. A simplex is a geometrical figure in N dimensions containing N + 1 points. For the image density function defined above, N has the value 9. In two dimensions, for example, a simplex will contain 3 points, with lines connecting each pair of points. This simplex is called a triangle. As the dimension increases, the complexity of the simplex also increases. In three dimensions a  
25 simplex is a tetrahedron. This implies that if there are N parameters to be optimized, then N + 1 solutions must be maintained. This translates to N<sup>2</sup> + N storage locations that are required to run the algorithm.

For exemplification, the optimization problem with 2 parameters is as follows. The simplex, a triangle, is formed from three points or three different  
30 sets of values for the parameters. These three points (call them solutions A, B and C), which are generated in the following way. Starting with an initial set of parameters (solution A), each parameter is perturbed by a small amount

-52-

(typically 0.01). When the first of the two parameters is changed, solution B is generated. When the second parameter is perturbed, solution C is generated. The three solutions must be evaluated to determine the error function value for each.

- 5            Suppose that solution A has the highest error function value. The simplex algorithm attempts to make an improvement by picking a new point (solution, or set of parameters), that lowers the error function value. This basic operation is called a reflection. Three attempts are made at improving the solution. The first, normal, reflection picks its new set of parameters by
- 10 forming a line from point A to the average of the remaining points. The line is then extended through the average point an equal distance. This new point is the reflection point. Reflection is the correct term since if one were to place a mirror on the line between B and C, the new point corresponds exactly to the reflection of A in the mirror.
- 15            If the new error function value for the normal reflection is better than the best current solution, then an expansion reflection is attempted. In this case the line from A is extended by the Step Up Factor (typically 1.50) through the average point. This operation makes the simplex larger. The point that gave the best error function value (either the normal reflection of A or the Expansion
- 20 reflection of A) is retained as the new A point.
- If the new error function value for the normal reflection is still the worst solution, then a contraction reflection is attempted. In this case the line from A is extended by the Step Down Factor (typically 0.75) through the average point. This operation makes the simplex smaller. If this solution is better then the
- 25 original error function value for point A, the reflection point is retained as point A. If no improvement is made in the A solution, then the entire simplex is contracted by moving each point toward the point with the best error function value by the fraction specified by the Shrink Factor (typically 0.95). These reflection operations continue until the difference between the best and worst
- 30 solutions falls below the Restart Tolerance (typically  $1.0E-9$ ).

**Alternative Method 1 for R Reducing the Image to Parameters Using a Neural Network**

-53-

A neural network can be used as an alternative to a polynomial mathematical function for the purpose of generating parameters that can be used to reconstruct an image. The basic architecture of the neural network contains at least three processing layers. During the training process, a  
5 sequence of example images are presented to the network for training. Training continues so that the error between each image and its reconstruction is minimized across the set of images used for training. The image, or a subsection of the image, is presented to the input layer of the network. The middle layer, or hidden layer, of the network contains a number of processing  
10 element that is much smaller than the number of inputs in the input layer. The output layer contains the same number of processing elements as the input layer. The output layer of the network will represent the reconstructed image that is presented to the input layer.

An alternative architecture contains an odd number of hidden layers,  
15 with the middle hidden layer containing a much smaller number of processing elements than the input and output layers. In each layer of the network, each processing element is connected to each of the processing element outputs of the previous layer.

The processing element used in the network typically generates a  
20 weighted sum of the inputs to processing element, with a transfer function applied to the weighted sum to generate the output of the processing element. The transfer function is any such function normally used in a neural network, including the sigmoid function, or the hyperbolic tangent function.

The neural network can be trained using any standard neural network  
25 training rule, including the back propagation learning rule. At each step of the training process, a training image is presented to the inputs of the neural network. The same image is also be presented to the outputs of the network as the desired, or target, output of the network. As learning proceeds, the error between the outputs of the neural network and the desired outputs of the  
30 network decreases.

In order for the error to decrease, the neural network middle hidden layer generates a greatly reduced representation of the input image that contains

-54-

enough information to reconstruct the image. This reduced representation therefore also contains the information needed to classify the image.

Once trained, a new image is presented to the inputs of the neural network. The outputs of the middle hidden layer are then be used as the inputs  
5 to the classification means for further processing.

**Alternative Method 2 for Reducing the Image to Parameters Using a Neural Network**

A second alternative method for reducing an image to useful parameters is to substitute the neural network directly in place of the polynomial  
10 mathematical function. Here, the inputs of the neural network are the coordinates of the pixel in the image being examined. The desired output of the network are the density value of the associated pixel.

The architecture of this neural network is substantially smaller then the architecture described in the first alternative method. Here the weights of the  
15 neural network become the parameters to be used by the classifier. The types of processing elements used in this architecture include the radial basis function type, and provisions might be made to allow a mix of processing element types in the hidden layer of the neural network. The architecture is developed to provide the smallest possible number of weights while still being capable of  
20 reconstructing the image.

In this alternative, the neural network is trained only on the image under consideration. Thus, each time a sample is tested, the network would be retrained. The weights of the trained network are used as inputs to the classification means.

25 **Assay Validation**

**Method for Classifying the Image from the Parameters**

Once the parameters are estimated, the parameters generated from the image reconstruction process along with several parameters easily calculated from the scanned image are used to classify the sample. In addition, the image  
30 parameters from several reference scans are used. The process of classification incorporates two steps. The first is a validation step to determine if the sample



-55-

under consideration should be rejected or classified. The validated result is then classified as positive or negative as described above.

To ensure the accuracy of a test result, the system producing that result should be validated. Validation protocols are used to confirm that all

- 5 components of a system operate properly, and that the data received from the system is meaningful. Moreover, in systems where raw data from instruments are manipulated by software, the proper functioning of that software should also be validated.

- Validation of data analysis software can be performed in any number of  
10 ways. Typically, a known sample (e.g., reference, positive control, negative control) can be tested in the system to confirm that the expected result is obtained. Alternatively, known raw data can be stored in memory and acted upon by the data analysis software to confirm that the expected result is obtained. Such validation protocols ensure that the software is operating  
15 properly before a clinical sample of interest is evaluated in that system.

- Validation of test systems can also be performed during the evaluation of a clinical sample being tested by that system. These types of validation protocols can evaluate components of the system, either individually or together. When the criteria set by assay validation protocols are not achieved,  
20 an invalid result is obtained, and the user will be made aware of the system malfunction. Such processes ensure that only accurate test results are presented to the user.

- In an exemplary embodiment, for example, data are validated by several methods. First, the data are checked for completeness by checking that the  
25 size of the matrix is  $m \times n$ , where  $m$  is the number of columns of data collected (e.g., location on dipstick, dark reading, reflectance at  $\lambda_1$  and reflectance at  $\lambda_2$ ) and  $n$  is the number of steps, or readings, taken along the test strip. For example, in the preferred embodiment, the matrix must be of an exact size of  $4 \times 226$ .

- 30 The extent of color development at the control line may also be used to validate that each assay ran properly. For example, quantitation of the control peak height, or area, may be used as assay validation criteria. Specifically, an

-56-

assay validation criterion might be imposed such that only those scans that yield a control peak height of greater than or equal to a specified value, determined empirically for the assay in question, will be valid, otherwise the scan is rejected. For example, in a particular embodiment, where fFN is

- 5 detected on an immunoassay test strip, as described herein, the control peak height must be greater than 0.05 intensity units.

**Method for generating controls for assays and the resulting controls**

- A method for generating controls and the resulting controls are provided herein. This method is based upon the observation that some systems generate
- 10 data that are conducive can be modelling (i.e., fitting). Empirical analysis will determine construction of an algorithm such that valid data are modelled accurately, while invalid data are difficult to model. For example, if it is known that a scan by the reader (intensity versus distance along the strip) should be relatively flat except for two normally distributed peaks in the central region. , It
- 15 has been found that the curve is composed of a linear, or parabolic, function to estimate the baseline, a first gaussian function to estimate one of the peaks, and a second gaussian function to estimate the other peak. Such a composite function would readily fit scans generated during normal operation, but would not fit well scans generated during abnormal operation. Under these types of
- 20 conditions, the comparison of the fitted image with the original image may serve as another criteria for assay validation.

- More specifically, if the linear regression of the fitted versus original image were solved, the r-square value and the slope of the linear regression may serve as assay validation criteria. Thus, based on historical empirical data
- 25 obtained from other runs on similar samples, upper and lower limits on r-square and slope would be set such that scans which do not fit within the limits within a specified number of attempts to optimize the fit are rejected. For example, assay validation criteria might include a requirement that r-square be greater than or equal to 0.97. The particular value is dependent upon the test and will
- 30 be determined by the skilled practitioner. Moreover, another assay validation criteria might include a requirement that the slope of the linear regression must be between 0.98 and 1.10, inclusive. Again the particulars of each determina-

-57-

tion are a function of the test, the type of data and results, and the tolerance for and amount of variation.

This method is advantageous in that it provides an internal validation, in contrast with other controls, which usually involve comparison of results  
5 against a previously established range, or against other test samples, such as positive or negative controls or reference samples. It is based on the concept that any assay can be controlled based on expected results.

For example, using the assay exemplified herein, where fFN is detected in the immunoassay, based upon repeated performance of the assay, it has  
10 been found that the expected reflectance data can be readily modeled by a composite curve comprised of a parabolic and two gaussian functions. Therefore, any time the assay is run, the resulting data should be modeled (fit) by the same composite curve. Knowing this, it is possible to identify scans, which although the positive and negative controls are show tha the assay  
15 worked, should be classified as invalid. Such scans (assay runs), for example, if they required a sigmoidal, rather than parabolic, baseline. would not readily fit (model) with the composite function, and would be classified as invalid. The failure to fit for example, could reflect defects in the test strip, or changes in the environment during the run, etc., that would affect the run, but might not affect  
20 the positive and negative controls.

If assay validation criteria have been met, then the result can be interpreted as either positive or negative by comparing the intensity of the test peak of the clinical sample with the intensity of the test peak of the positive reference. A test is positive if the intensity of the test peak of the clinical  
25 sample is greater than or equal to the intensity of the test peak of the positive reference. A test is negative if the intensity of the clinical sample is less than the intensity of the test peak of the positive reference. In calculating intensity, either peak height or peak area may be used.

#### 30 **Alternative Method for Classifying the Image Using a Neural Network**

Based on the available data generated from scans all possible variables were identified that could be used to improve the ability to classify the sample.

-58-

The initial training runs used the parameters generated from the image reconstruction process along with several parameters easily calculated from the scanned image. One such parameter is the area under a peak. It can be calculated from original parameters as following:

- 5           Area =  $\sqrt{\pi}$  \* Height / S, where S is spread or width of the peak. A sigma variable, related to the normal distribution can also be calculated from the parameters by:

$$\text{Sigma} = 1 / (\sqrt{2} * S).$$

- In addition, the image parameters from a Calibrator scan (fFN positive reference)  
10       were also used. The following is a list of the variables that are available for use by the neural network.

1. Sample Baseline Square Term
2. Sample Baseline Linear Term
3. Sample Baseline Offset
- 15       4. Sample Control Peak Position
5. Sample Control Peak Sigma
6. Sample Control Peak Area
7. Sample Test Peak Position
8. Sample Test Peak Sigma
- 20       9. Sample Test Peak Area
10. Sample Test Peak Height
11. Sample Control Peak Height
12. Sample Baseline estimated value between the peaks
13. Sample Ratio of Test Area to Control Area
- 25       14. Sample Ratio of Test Height to Control Height
15. Calibrator Baseline Square Term
16. Calibrator Baseline Linear Term
17. Calibrator Baseline Offset
18. Calibrator Control Peak Position
- 30       19. Calibrator Control Peak Sigma
20. Calibrator Control Peak Area
21. Calibrator Test Peak Position

-59-

- 22. Calibrator Test Peak Sigma
- 23. Calibrator Test Peak Area
- 24. Calibrator Test Peak Height
- 25. Calibrator Control Peak Height

- 5 26. Calibrator Baseline estimated value between the peaks
- 27. Calibrator Ratio of Test Area to Control Area
- 28. Calibrator Ratio of Test Height to Control Height

Four predictor variables were also added. In these variables the calibrator strip value is compared to the sample strip value and a +1 or -1 is used depending

- 10 on the comparison. The additional variables are:

- Test Area Predictor
- Area Ratio Predictor
- Test Height Predictor
- Height Ratio Predictor.

- 15 The desired, or target output of the neural network was a classification of the concentration of the sample. If the sample concentration was greater than or equal to 50 ng/ml the desired output was set to 1.0. The desired output was set to 0 otherwise. A sensitivity analysis of the associated training runs was used to indicate which variables were important to the prediction task. The

- 20 ThinksPro software product from Logical Designs Consulting was used to train the networks and perform the sensitivity analysis. Alternatively, a variable selection process based on genetic algorithms or some other method could be used to select the best subset of variables from this list (see, e.g., copending U.S. application Serial Nos. 08/798,306 and 08/912,133, which describe a
- 25 suitable variable selection process).

Using the reduced set of variables one or more networks are trained to estimate the classification of the sample. If more than one network is used, the outputs of each network are averaged together to give a consensus result.

- In another embodiment, the nine variables may optionally be fed through
- 30 a previously trained neural network to obtain a test result. For example, the nets may be trained with data for which ELISA test results are known. Alternatively, variables other than the nine described above may be used to

-60-

train the neural net. The nets can be used not only to return positive or negative results, but also to determine if the assay itself is valid for any particular run.

The reduction of data for input to neural networks can be accomplished  
5 by a neural network itself. An example of such a net is a net with an hourglass architecture with an input, output and three hidden layers, wherein the input and output layers contain  $n$  nodes, with the first and third hidden layers containing less than  $n$  nodes, and the second hidden layer containing five  
10 nodes. If trained so that the output layer exactly matches the input layer, such nets would reduce the original dataset of  $n$  elements down to five elements, and also retain the ability to reconstruct the original dataset of  $n$  elements from these five elements.

#### Further Analysis Using Decision Support Systems

The output from the data analysis step provides an assessment of the  
15 raw biochemical test data that is measured by the reader or other instrument. Such data may then be considered as is, but it can be further entered into a decision-support system, particularly a neural network, that has been trained to evaluate the particular data and disease. For example, U.S. application Serial No. 08/599,275, now abandoned, copending U.S. application Serial No.  
20 08/798,306, and copending U.S. application Serial No. 08/912,133, filed 8/14/97, as well as published International PCT application No. WO 97/29447 and International PCT application No. PCT/US98/16891, which claims priority to U.S. application Serial No. 09/134,636 and U.S. application Serial No. 08/912,133. PCT application No. WO 97/29447 claims priority to U.S.  
25 application Serial No. 08/599,275, filed 2/9/96, now abandoned, and copending U.S. application Serial No. 08/798,306. These documents provide neural nets and methods for developing neural networks for diagnosis of disorders that can be used in the systems as provided herein.

The accuracy of biochemical test data is improved when used in these  
30 neural nets. Such neural nets, are thus contemplated for inclusion in the systems herein.

-61-

Briefly, in the methods described in these applications patient data or information, typically patient history or clinical data, are analyzed by the decision-support systems to identify important or relevant variables and decision-support systems are trained on the patient data. Patient data are

5 augmented by biochemical test data or results to refine performance. The resulting decision-support systems are employed to evaluate specific observation values and test data to guide the development of biochemical or other diagnostic tests, to assess a course of treatment, to identify new diagnostic tests and disease markers, to identify useful therapies, and to provide

10 the decision-support functionality for the test. Methods for identification of important input variables for a medical diagnostic tests for use in training the decision-support systems to guide the development of the tests, for improving the sensitivity and specificity of such tests, and for selecting diagnostic tests that improve overall diagnosis of, or potential for, a disease state and that

15 permit the effectiveness of a selected therapeutic protocol to be assessed are also provided. The methods for identification can be applied in any field in which statistics are used to determine outcomes. A method for evaluating the effectiveness of any given diagnostic test is also provided.

Thus, such neural networks or other decision-support systems will be

20 included in the systems provided herein as a means of improving performance of the biochemical test data.

The following examples are included for illustrative purposes only and are not intended to limit the scope of the invention.

#### EXAMPLE 1

##### 25 Immunoassay Test Strip

###### A. The Test Strip

The test strip 100 includes a membrane system including three components: a porous or bibulous member 102; a conjugate pad 108; and an absorbent pad 110. The membrane system may be mounted on a substrate or

30 backing 112, with the conjugate pad 108 and the absorbent pad 110 slightly overlapping the porous or bibulous member 102, which is interposed thereinbetween. As can be seen, the conjugate pad 108 overlaps the porous or

-62-

bibulous member **102** so that a fluid sample placed onto the conjugate pad **108** is communicated from the conjugate pad **108** to the porous or bibulous member **102**. Similarly, the absorbent pad **110** overlaps with the porous or bibulous member **102** so that fluid samples introduced into the porous or bibulous member **102** from the conjugate pad **108** can then be transmitted to the absorbent pad **110**. Thus, the conjugate pad **108**, the absorbent pad **110** and the porous or bibulous member **102** are all in fluid communication with one another, making any fluid sample placed on the conjugate pad **108** able to propagate through the conjugate pad **108** to the porous or bibulous member **110** and then to the absorbent pad **110**.

The porous or bibulous member is capable of transporting a liquid sample along the test strip and serves as the solid support upon which the immunoreactions occur. Antibodies which react with the target analyte and/or label are immobilized on the solid support. Possible solid supports include paper and cellulose derivatives, such as cellulose esters and ethers, natural and synthetic polymeric materials, such as vinyl polymers and partially hydrolyzed derivatives, polycondensates, copolymers and inorganic materials. A preferred solid support is a nitrocellulose membrane.

The porous or bibulous member contains two distinct zones, a detection zone **104** and a control zone **106**, at which two different antibodies are immobilized. The detection zone contains an immobilized capture antibody that binds the analyte of interest, whereas the control zone contains an immobilized antibody or other component, such as an antigen, that binds labeled antibody conjugate (discussed below) which has not bound to analyte.

The membrane system also includes a conjugate pad **108**, which serves as a sample application component, and which includes an antibody to the analyte, which is conjugated to a detectable label. The conjugate pad is in fluid communication with the porous or bibulous member **102**. The labeled antibody conjugate is diffusively bound to the conjugate pad and becomes mobile upon application of the liquid sample and moves along the test strip. The conjugate pad is made of a porous material, such as glass fiber. The conjugate pad may also act as a pre-filter for the sample.



-63-

The membrane system may also include an absorbent pad 112, which is also in fluid communication with the porous or bibulous member, and which serves to draw liquid continuously through the device. The absorbent strip may be made of a material such as cellulose paper or other material known to those of skill in the art.

Referring to FIG. 2A, which depicts an exemplary immunoassay device, including a test strip and housing assembly 200, the housing 202 generally surrounds the test strip 100 (FIG. 1) and includes an opening through which test sample is applied 204, as well as an aperture above the detection and control zones 206 that permits measurement of the amount of label by the reader, which is correlated with the amount of analyte in the test sample. The housing 202 includes at its upper surface 208 a fattened end 210, used for gripping the housing 202, an application window 204 (or sample window) through which a sample is applied to a conjugate pad 108 of an immunoassay test strip within the housing 202. The housing 202 also includes a test window 214 through which the test result of the immunoassay is viewed. In accordance with the embodiments shown, no window material is mounted within the test window 214 (or the sample window 212). Thus, an optical path from outside the housing 202 through the test window 214 to the immunoassay test strip is unobscured by even a transparent material. Other alternative embodiments may include an optically transparent material (transparent at wavelengths emitted by light emitted from devices described herein), however, such is not preferred. Also, as shown in FIG. 2A and FIG. 2B, the housing may include a symbology, exemplified as a bar code 216 or 316 that can be read by the reader or a separate reading device and associated with identifying information pertaining to the particular device and/or test run or other information.

An alternative embodiment of the test device is shown in FIG. 2B. The components of device are shown in FIG. 3 and include the upper and lower members 302 and 304 of the housing and the test strip 100. Also shown are the sample application port 306, test window 308, and the optionally included bar code 316.

-64-

Referring next to FIG. 4 a top view is shown of the immunoassay test strip housing 202 of FIG. 2A. Shown are the sample window 212, and the test window 214, and the enlarged gripping portion 210. Also shown are structures 402 for holding the immunoassay test assembly within the housing 202 and  
5 structures 404 for securing upper and lower halves of the housing 202 to one another.

Referring next to FIG. 5, a side cross-sectional assembly view is shown of the housing 202 for the immunoassay test strip 100. Shown are the sample window 212, the test window 214, and the structures 402 for holding the  
10 immunoassay test strip assembly in place within the housing 202. As can be seen, an upper half 502 of the housing 202 is mated with a lower half 504 of the housing 202. The immunoassay test strip is sandwiched between the upper and lower halves 502 and 504 of the housing 202 and is secured in place by the structures 402 of the upper half 502. The immunoassay test strip is  
15 positioned so as to be viewable through the test window 214 when the immunoassay test strip assembly is secured within the housing and the conjugate pad is positioned to be contactable through the sample window 212.

These devices are particularly adapted for use with the reflectance reader provided herein.

20        **B.        Colored Latex Label and assays using the latex label**

The immunoassay test strip includes a membrane system supported on a plastic backing. The membrane system is formed from three partially overlapping materials: a conjugate pad made of Whatman glass fiber (F075-07S, 2.4 cm length) treated with polyvinyl alcohol (PVA), a nitrocellulose strip  
25 supplied by Sartorius (8  $\mu$ m, 3.3 cm length) and an absorbent pad made of Whatman C7218 (1.65 cm length) cellulose paper. These three materials are in fluid communication with each other. The conjugate pad and nitrocellulose overlap by 1 mm and the nitrocellulose and absorbent pad overlap by 4 mm. The membrane materials are hand-laminated and attached to a membrane card,  
30 which is cut using an Azco guillotine compression cutter, using G&L adhesive membrane.

-65-

The conjugate pad contains a mouse monoclonal anti-fFN antibody (FDC-6 or A137) conjugated to latex particles containing a blue dye. The conjugate pad acts as a pre-filter for the sample in that mucous from the sample is left behind in the conjugate pad after performing the assay.

- 5        The latex particles, which are polymerized from styrene and acrylic acid, may be any suitable latex particles (such as are available from Bangs Laboratories). The particles are polymerized in an aqueous solution with a surfactant added. The particles are internally labeled with blue dye by swelling the particles in organic solvent and adding the dye. The particles are then  
10   placed in an aqueous solvent, which shrinks the particles and traps the dye. The dye is an organic soluble blue dye. Carboxyl groups are covalently attached to the surface of the bead for coupling to the antibody. The particles (Bangs Uniform Microsphere Stock D0004031CB) are supplied as a 2.5-10% aqueous suspension containing surfactant and have a mean diameter of 0.40  
15    $\mu\text{m}$ , with a standard deviation of 0.4  $\mu\text{m}$ , and a surface area of  $1.405\text{e}+13$   $\mu\text{m}^2/\text{g}$ .

- Antibodies are conjugated to the latex particles in a one-step covalent conjugation process using EDAC, a carbodiimide coupling reagent. The conjugate is characterized as approximately 1% solids; 50  $\mu\text{g}/\text{mg}$  beads total  
20   bound protein (Bead BCA); and greater than 50%, preferably 80%, covalent bound protein (Tris-SDS + Bead BCA).

- The antibody conjugated to the latex particles is mouse monoclonal antibody specific for fetal fibronectin. The antibody (FDC-6 or A137 monoclonal, deposited at the American Type Culture Collection as accession  
25   number ATCC HB 9018( see U.S. Patent No. 4,894,326) is raised against whole molecule onco-fetal fibronectin from a tumor cell line. The antibody is produced as ascites and is purified by Protein G and dialyzed into PBS buffer.

- The nitrocellulose strip contains two distinct zones, a detection zone and a control zone, at which two different antibodies are immobilized. The  
30   detection zone contains immobilized anti-fibronectin polyclonal antibody as a capture antibody, whereas the control zone contains immobilized goat anti-mouse polyclonal antibody. The anti-fibronectin polyclonal antibody is produced

-66-

- in goats. The antisera is obtained from a commercial source and is purified by use of a fibronectin column which is made by attaching purified fibronectin (antigen) to a resin. The antisera is passed through a column containing the resin. After washing unbound material, the antibody is eluted via low pH
- 5 glycine. The purified antibody is then dialyzed. The purified goat anti-mouse IgG antibody (GAMGG) immobilized in the control zone is obtained from a commercial source (e.g. Biosource) or can be prepared, if desired, e.g. by passing the serum through a mouse IgG column, which binds the antibody, and then eluting off the antibody using glycine, or by any suitable method.
- 10 The antibodies are applied to the conjugate pad and nitrocellulose strip using an IVEK Linear Stripper, which is a volumetric ceramic piston pump dispenser. The anti-fibronectin polyclonal capture antibody is applied in a 1x Spotting Buffer P/N 00387, which contains citrate, phosphate and NaCl, at an antibody concentration of 1 mg/ml and a striping rate of 1  $\mu$ l/sec. The position
- 15 of the test line is about 37-40 mm, preferably 38-39 mm, from the bottom of the strip. The control antibody is applied in a 1x Spotting Buffer P/N 00387 at a concentration of 0.5 mg/ml and a striping rate of 1  $\mu$ l/sec. The position of the control line is approximately 43-46 mm, preferably 44.5-45.5 mm, from the bottom of the strip. The dimensions of the antibody stripes are approximately
- 20 8.1 mm (wide) x 0.5-1.0 mm (high), or any other suitable size. The nitrocellulose strip is not otherwise treated after application of the capture and control antibodies to block non-specific binding sites.

- The detection and control stripes are applied to the strip and then dried for at least 24 hours at RT, after which the conjugate is striped onto the strip.
- 25 The conjugate is mixed in a diluent containing 20% sucrose, 0.2% BSA, 0.05% TW20 and 0.05% sodium azide in 100 mM Tris. After application of the conjugate, the strip is then dried, preferably for 30 minutes at 37°C, or at least 24 hours at RT, or the equivalent thereof.

- The test strip is contained within a housing, which includes a lower
- 30 member and an upper member with openings that include a circular aperture above the area of the conjugate pad, through which test sample is applied, and a rectilinear aperture above the detection and control zones. The circular

-67-

application aperture is in contact with the test strip. The latex conjugate is placed slightly downstream from the sample application opening. The upper and lower members are mated together to sandwich the test strip. The test strip is confined non-removably in the housing, and the device is not intended to be re-usable. The upper member is configured for use with a reader that measures the amount of label that is indicative of the amount of fetal fibronectin in the test sample.

**C. Colloidal Gold Label and assays using colloidal gold label**

In an alternative embodiment, colloidal gold is used for labeling the antibody. The test strip configuration is similar to that described in EXAMPLE 1A for the latex particle embodiment, with the following modifications.

In the colloidal gold assay, a goat polyclonal antibody to human adult and fetal fibronectin is present in the conjugate pad, immobilized mouse monoclonal anti-fetal fibronectin antibody (specific to the III CS region of fetal fibronectin) is present in the detection zone of the nitrocellulose test strip and immobilized human adult fibronectin is present in the control zone.

The anti-fibronectin antibodies (polyclonal) are labeled with colloidal gold by passively adsorbing anti-fibronectin antibodies onto colloidal gold. This preparation is then treated with a solution containing protein and polyvinyl pyrrolidone (PVP) to coat the colloidal gold particles. This method is described in Geoghegan and Ackerman, Journal of Histochemistry and Cytochemistry, 25(11):1187-1200 (1977).

**EXAMPLE 2**

**Immunoassay Procedure**

**A. Colored Latex Label**

In conducting the assay, the sample is extracted from a swab into antiprotease transfer buffer (0.05 M Tris buffer, pH 7.4, 1% BSA, 5 mM EDTA, 1 mM phenylmethylsulfonyl fluoride (PMSF), and 500 Kallikrein Units /ml of Aprotinin), heated for 15 minutes at 37°C and filtered through a large pore (25  $\mu$ ) plunger filter. A volume of 200  $\mu$ l of test sample is then delivered to the conjugate pad at the application zone using a standard plastic pipet. Any fFN in the sample will bind to the labeled monoclonal antibody and the resulting

-68-

complex migrates into the nitrocellulose strip. When the complex encounters the detection zone, the immobilized anti-FN antibody binds the complex, thereby forming a colored stripe due to the accumulation of the dye-containing latex beads. Any unbound latex-conjugated anti-fFN antibody continues to migrate  
5 into the control zone where it is captured by the immobilized goat anti-mouse antibody and thereby forms a colored stripe due to the accumulation of the dye-containing latex beads. The reaction time is 20 minutes.

#### B. Colloidal Gold Label

The test strip assay procedure is similar to that described in EXAMPLE  
10 2A for the latex particle embodiment, with the following modifications. The buffer used to extract the sample is Tris-acetate and a protein matrix (4% PSA and 4% PVP).

Fetal fibronectin and adult human fibronectin in the sample bind with the labeled anti-fibronectin antibody conjugate on the conjugate pad. The labeled  
15 fetal fibronectin-anti-fibronectin complex and adult human fibronectin-anti-fibronectin complexes, and unbound labeled anti-fibronectin conjugate migrate into the nitrocellulose strip, where they encounter the detection region, including immobilized anti-fetal fibronectin monoclonal antibody.

In the detection region, the immobilized anti-fetal fibronectin capture  
20 antibody binds with the fetal fibronectin-anti-fibronectin complex, whereby a gold label forms a colored stripe due to concentration of the gold label. The amount of gold label bound to the test region correlates with the amount of fetal fibronectin in the sample.

The unbound labeled anti-fibronectin antibody conjugate and adult human  
25 fibronectin-anti-fibronectin complex then pass to the control region of the immunoassay test strip, which includes immobilized adult human fibronectin. There, any unbound antibody conjugate binds to the immobilized adult human fibronectin, where the gold label forms a second colored stripe. The presence of a colored stripe indicates that the assay results are valid, whereas the  
30 absence of this stripe indicates that the results are not valid, i.e., that the sample did not reach the control region, and thus a good reading at the test

-69-

region cannot be assumed. Any adult human fibronectin-anti-fibronectin complexes formed do not bind with the detection or control zones.

### EXAMPLE 3

#### Operation of the Reflectance Reader

- 5           The test strip is read using the reflectance reader exemplified herein. This reader (described above) is adapted to read an immunochromatographic test strip supported within the housing. The reflectance reader includes a cassette slot for receiving the test-strip housing, and a sensing head assembly for reading the test strip supported within the test-strip housing using reflected
- 10 light. The sensing head assembly includes a first light-emitting diode (LED<sub>1</sub>), a second LED (LED<sub>2</sub>), a silicon photodiode detector, and 39 optical fibers randomly arranged in a narrow slit (e.g., 0.020" wide) located at the bottom of the sensing head assembly. LED<sub>1</sub> emits light with a wavelength of 430 nm (blue), and LED<sub>2</sub> emits light with a wavelength of 595 nm (amber). The optical
- 15 fibers are arranged in three groups of 13 optical fibers each: the first group transmits light emitted by LED<sub>1</sub> to the slit; the second group transmits light emitted by LED<sub>2</sub> to the slit; and the third group transmits reflected light received at the slit to the photodetector. The 39 fibers each include an end randomly arranged within a plane located at the slit such that the ends are co-planar, with
- 20 the plane being normal to the test strip when the sensing head assembly is positioned (as described below) to take reflectance readings. The optical fibers in each of the three groups are randomly arranged within the plane with respect to the fibers of the other two groups.

- The slit width is selected to be as narrow as permitted, with the practical
- 25 minimum being driven by the availability of small diameter optical fibers. The maximum slit width should not be larger than about 90% of the width of the colored stripe, otherwise the background of the strip, in addition to the colored stripe, will be read and less color will be detected, unless the slit, or aperture, is positioned directly above the colored stripe.

- 30           When the housing is inserted into the cassette slot of the reader, a spring mechanism rotates the sensing head directly over the second aperture of the housing such that the plane defined by the optical fibers is normal to the

-70-

surface of the nitrocellulose strip at a distance of about 0.010". Light from LED<sub>1</sub> and LED<sub>2</sub> can be transmitted by the fibers onto the nitrocellulose strip at a normal angle, and light reflected normally from the strip can be transmitted by the fibers to the photodetector.

- 5           The sensing head takes three separate reflectance readings of each portion of the nitrocellulose strip by reading the output of the photosensor while controlling LED<sub>1</sub> and LED<sub>2</sub>. The first reading, used to determine the amount of ambient light leaking into the reader (e.g., light leaking through the slot entrance, or light reflected into the reader through the white plastic of the
- 10 housing), is a dark reading taken with LED<sub>1</sub> and LED<sub>2</sub> both turned off. The dark reading count is subtracted from the other two readings to correct for light leakage. The second reading, used to determine background reflections associated with the nitrocellulose, is taken with LED<sub>1</sub> pulsed on and LED<sub>2</sub> turned off. The third reading, used to detect the presence of the latex label on the test
- 15 strip, is taken with LED<sub>2</sub> pulsed on and LED<sub>1</sub> turned off. A control circuit reads the photodetector output and controls the on and off operation of LED<sub>1</sub> and LED<sub>2</sub>. A memory circuit stores the raw and/or processed data. The data may also be displayed to the operator via an appropriate interface (e.g., an alphanumeric character matrix).
- 20           After being positioned above the housing by the spring mechanism, the sensing head can be moved slidably across the test strip to allow the head to scan the entire exposed surface of the nitrocellulose strip (including the detection and control zones). In the preferred embodiment, this distance is approximately 0.452". The head is slidably connected to a rail (e.g., guide
- 25 rods), and is coupled to a worm or screw gear driven by a stepper motor. Under the control of the control circuit, the stepper motor drives the head along the rail in small steps (e.g., 0.002"/step). At each step, the control circuit takes three readings as described above. Thus, the control circuit moves the head such that the optical fibers pass directly above and normal to the exposed
- 30 surface of the nitrocellulose strip in a sequence of small steps, and takes a sequence of dark, LED<sub>1</sub> and LED<sub>2</sub> readings at each step. The control circuit then



-71-

processes the data read from the photodetector at each sequence of three readings to determine the presence or concentration of fFN.

Since the detection and control latex stripes are each about 0.020" wide, and since each step of the sensing head is about 0.002" long, there will  
5 be about 10 steps within each stripe. Thus, there will be 10 sets of three readings (i.e., dark, LED<sub>1</sub> and LED<sub>2</sub>) at each of the stripes, and the remainder of the reading sets will not be made over either stripe.

The control circuit processes the LED<sub>1</sub> and LED<sub>2</sub> readings by first subtracting the "dark reading" taken at the corresponding step to correct for  
10 light leakage. The corrected LED<sub>1</sub> and LED<sub>2</sub> readings are then input into a ratiometric algorithm to determine the concentration of fFN. The algorithm is based upon the ratio of readings at the detection and control zones. If a sample includes a high concentration of fFN, latex readings at the detection zone will be relatively high and the readings at the control zone will be low. If the sample  
15 includes a low concentration of fFN, however, latex readings at the detection zone will be relatively low and readings at the control zone will be high. The algorithm calculates a reflectance ratio for each step which equals (amber count - dark count)/ (blue count - dark count). Generally, light leakage is so minimal that this step can be omitted. If the reflectance ratio is graphed as a function of  
20 the steps, the result will be a two-peak graph with the peaks occurring at the two stripes. The graph is mathematically analyzed, with a sigmoidal calculation across the background and a gaussian calculation to integrate the area beneath each of the two peaks. The fFN concentration is then determined based upon the ratio of the integrated area beneath each of the two peaks.

25 In operation, when the test-strip housing is inserted into the cassette slot of the reader, the sensing head rotates down over the exposed nitrocellulose strip, and the control circuit then moves the head to an initial position. The control circuit moves the head across the exposed surface of the nitrocellulose strip, including the detection and control zones, in small increments of 0.002"  
30 each. At each step, the control circuit takes a first reading of the photodetector output with LED<sub>1</sub> and LED<sub>2</sub> both off, takes a second reading with LED<sub>1</sub> pulsed on and LED<sub>2</sub> off, and takes a third reading with LED<sub>1</sub> off and LED<sub>2</sub> pulsed on.

-72-

The control circuit then steps the sensing head and repeats the three readings. This process is repeated for each of 226 steps (0.452" at 0.002"/step) until the entire surface is read. The control circuit may then analyze the raw data to determine the presence or concentration of fFN. The output values can be  
5 displayed via an operator interface, or can be output to another computer or apparatus.

Since modifications will be apparent to those of skill in this art, it is intended that this invention be limited only by the scope of the appended claims.

-73-

**CLAIMS:**

1. A point of care system for determining results from a diagnostic or risk assessment test, comprising:
  - a point of care test;
  - 5 a reader for analyzing data from the test; and
  - software programmed for analyzing the results from the test.
2. The point of care system of claim 1, wherein the reader is a reflectance reader with a reader head that comprises:
  - a reader head body;
  - 10 a light emitting diode;
  - a first fiberoptic bundle optically coupled to the light emitting diode;
  - a photodetector;
  - a second fiberoptic bundle optically coupled to the light
  - 15 photodetector;
  - an aperture in the reader head body;
  - a plurality of fiberoptic conductor ends arranged in a sigmoidal distribution in the aperture, a first portion of the fiberoptic conductor ends being of fiberoptic conductors of the first fiberoptic bundle, and a second portion of
  - 20 the fiberoptic conductor ends being of fiberoptic conductors of the second fiberoptic bundle.
3. The system of claim 1, wherein the point of care test includes a test strip that displays results from the test, and the reader is adapted to read the strip.
- 25 4. The point of care system of claim 1, wherein the reader is a reflectance reader, comprising:
  - a reader head comprising:
    - a reader head body;
    - a light emitting diode;
    - 30 a first fiberoptic bundle optically coupled to the light emitting diode, and adapted to transmitting light from the light emitting diode;

-74-

a photodetector adapted for generating a reflection signal in response to reflected light;

a second fiberoptic bundle optically coupled to the light photodetector, and adapted to transmit an amount of reflected light to the  
5 photodetector;

an aperture in the reader head body; and

a plurality of fiberoptic conductor ends arranged in a sigmoidal distribution in the aperture, a first portion of the fiberoptic conductor ends being of fiberoptic conductors of the first fiberoptic bundle, and a second portion of  
10 the fiberoptic conductor ends being of fiberoptic conductors of the second fiberoptic bundle, the plurality of fiberoptic conductor ends being further arranged in a substantially co-planar relationship; and

a reader housing comprising:

a housing body; and

15 a cassette slot adapted to receive a test device.

5. The system of claim 1, wherein the reader comprises:

a control unit including a processor modified with a software subsystem, wherein the software is for analyzing the data produced in the test.

6. The system of claim 4, wherein the reader further comprises:

20 a control unit including a processor modified with a software subsystem, wherein the software is for analyzing the data produced in the test.

7. The system of claim 1, wherein in the point of care test is an immunoassay.

8. The system of claim 1, wherein the test assesses the risk of  
25 having a condition or diagnoses the condition.

9. The system of claim 1, wherein the condition is pregnancy-related or the test assesses fertility status.

10. The system of claim 1, wherein the condition is infertility-related, a neurological disorder, a cardiovascular disorder, an inflammatory disorder, a  
30 viral or bacterial infection, a hormonal disorder, a metabolic disorder or a genetic disease.

-75-

11. The system of claim 1, wherein the results of the test are qualitative.
12. The system of claim 1, wherein the results of the test are quantitative.
- 5 13. The system of claim 1, wherein:  
the test is an immunoassay test strip, wherein the results from the immunoassay are detectable by a change in color or other property that can be detected using a reflectance reader; and the reader is a reflectance reader.
- 10 14. The system of claim 13, wherein the immunoassay test strip comprises:  
(a) a conjugate pad which serves as a sample application component;  
(b) a porous or bibulous member which is capable of transporting a liquid sample along the test strip and serves as the solid support upon which  
15 the immunoreactions occur; and  
(c) an absorbent pad, which serves to draw liquid continuously through the device, wherein:  
the materials of the membrane system form a single fluid flow pathway and the test strip is designed to be read by the reader.
- 20 15. The system of claim 14, wherein the porous or bibulous member comprises an immobilized capture antibody that binds to the analyte of interest in a detection zone.
16. The system of claim 8,  
wherein:  
25 the conjugate pad comprises an antibody diffusively bound thereto;  
the antibody is bound to a target analyte and is labeled with a colorimetrically or fluorometrically detectable label.
17. The system of claim 1, wherein the reader is a reflectance reader.
18. The system of claim 17, wherein the reflectance reader  
30 comprises:

-76-

data processing software employing data reduction and curve fitting algorithms converting the reflectance signal obtained from reading the test strip into a determination of the presence of an analyte in a sample.

19. A method for determining results from an immunoassay,  
5 comprising:

- (a) testing a patient sample for the presence of the a target analyte indicative of a condition or risk of having the condition by reacting the sample with an antibody specific for the analyte in a sandwich assay in which one of the antibodies is labeled with a colorimetrically detectable label;
  - 10 (b) detecting the signal produced by the assay in a reflectance reader, wherein the signal is indicative of the presence of the analyte; and
  - (c) processing the data obtained from the reflectance signals using data processing software employing data reduction and curve fitting algorithms and/or a trained neural network to convert the reflectance signal obtained from  
15 reading the test strip into a data indicative of the presence or absence or a threshold concentration of analyte in a sample.
- 20. The method of claim 19, wherein the results are qualitative.
  - 21. The method of claim 19, wherein the results are quantitative
  - 22. The method of claim 19, wherein the data is input into a neural  
20 network trained for assessing risk related to or diagnosing the condition.
  - 23. The method of claim 22, wherein the analyte is fetal fibronectin (fFN).
  - 24. The method of claim 23, wherein the condition is pregnancy-related or the immunoassay assesses fertility status.
  - 25. The method of claim 23, wherein the condition is an infertility-related disorder.
  - 26. The method of claim 23 that assesses the risk of ectopic pregnancy, pre-eclampsia, infertility, preterm labor, imminent delivery, term induction, fetal membrane rupture or infections of concern during pregnancy  
30 that may comprise the pregnancy or harm the newborn, including, for example, ascending genital infections such as chlamydia or herpes simplex virus.

-77-

27. The system of claim 7, wherein the immunoassay detects fetal fibronectin (fFN) in a sample.

28. A reflectance reader, comprising:

a reader head comprising:

5

a reader head body;

a light emitting diode;

a first fiberoptic bundle optically coupled to the light emitting diode;

a photodetector;

10

a second fiberoptic bundle optically coupled to the light photodetector;

an aperture in the reader head body;

a plurality of fiberoptic conductor ends arranged in a sigmoidal distribution in the aperture, a first portion of the fiberoptic conductor ends being  
15 of fiberoptic conductors of the first fiberoptic bundle, and a second portion of the fiberoptic conductor ends being of fiberoptic conductors of the second fiberoptic bundle.

29. The reader of claim 28, that is adapted for reading an assay test strip.

20

30. The reader of claim 28, further comprising software for correlating the reading with a diagnostic parameter.

31. The reader of claim 30, wherein the software comprises a decision-support system.

25

32. The reader of claim 30, wherein the software comprises a neural network.

33. The reader of claim 32 including the plurality of fiberoptic conductor ends arranged in a substantially co-planar relationship.

34. The reader of claim 28 further comprising:

another light emitting diode;

30

a third fiberoptic bundle optically coupled to the other light emitting diode;

-78-

a third portion of the fiberoptic conductor ends being of fiberoptic conductors of the third fiberoptic bundle.

35. The reader of claim 34 including a bonding agent between and around the fiberoptic conductors at the fiberoptic conductor ends, wherein the  
5 bonding agent maintains the fiberoptic conductor ends in said sigmoidal distribution.

36. The reader of Claim 35, wherein said light emitting diode is adapted to emit light of a first wavelength, and wherein said other light emitting diode is adapted to emit light of a second wavelength.

10 37. A method for reading the surface of a test strip comprising an image, comprising:

scanning the reader head in the reader of claim 1 to a first position over the surface comprising the image;

15 determining a first amount of light reflected from the surface comprising the image;

illuminating the surface for light of a first wavelength, and determining a second amount of light reflected from the surface;

illuminating the surface for light of a second wavelength, and determining a third amount of light reflected from the surface; and

20 determining a parameter correlated with the intensity or shape of the image.

38. The method of claim 37, wherein the parameter is the amount of an analyte in a sample, which is a function of the first amount of light reflected, the second amount of light reflected, and the third amount of light reflected.

25 39. The method of claim 37, wherein the method is for determining an amount of an analyte in a sample by correlating the reading with the amount of analyte in the sample.

40. The method of claim 37, wherein the surface comprises an assay test strip.

30 41. The method of claim 37, wherein illuminating with light of said first wavelength includes illuminating with light of said first wavelength, wherein said first wavelength is selected to reflect substantially equally from all



-79-

regions of the immunoassay test strip, whereby said second amount of light is indicative of the immunoassay test strip.

42. The method of claim 37, wherein illuminating with light of said second wavelength includes illuminating with light of said second wavelength, wherein said second wavelength is selected to reflect substantially optimally from the test region of the immunoassay test strip, whereby said third amount of light is indicative of an amount of label at the test region of the immunoassay test strip.

43. The method of claim 38, wherein the analyte is fetal fibronectin.

44. A reader head for use in determining an amount of analyte in a sample comprising:

a reader head body;  
a light emitting diode;  
a first fiberoptic bundle optically coupled to the light emitting diode;  
a photodetector;  
a second fiberoptic bundle optically coupled to the light photodetector;  
an aperture in the reader head body;  
a plurality of fiberoptic conductor ends arranged in a sigmoidal distribution in the aperture, a first portion of the fiberoptic conductor ends being of fiberoptic conductors of the first fiberoptic bundle, and a second portion of the fiberoptic conductor ends being of fiberoptic conductors of the second fiberoptic bundle, the plurality of fiberoptic conductor ends being further arranged in a substantially co-planar relationship.

45. A reflectance reader, comprising:  
the reader head of claim 44, wherein:  
the first fiberoptic bundle optically coupled to the light emitting diode is adapted to transmitting light from the light emitting diode;  
the photodetector is adapted for generating a reflection signal in response to reflected light;  
the second fiberoptic bundle optically coupled to the light photodetector is adapted to transmit an amount of reflected light to the photodetector; and

-80-

the plurality of fiberoptic conductor ends are arranged in a sigmoidal distribution in the aperture, a first portion of the fiberoptic conductor ends being of fiberoptic conductors of the first fiberoptic bundle, and a second portion of the fiberoptic conductor ends being of fiberoptic conductors of the  
5 second fiberoptic bundle, the plurality of fiberoptic conductor ends being further arranged in a substantially co-planar relationship

46. The reader of claim 45, further comprising:  
a reader housing comprising:  
a housing body; and  
10 a cassette slot adapted to receive a test device for measuring the analyte.

47. The reader of claim 45, that is for determining an amount of analyte in a sample

48. The reader of claim 45, wherein the test device is an  
15 immunoassay device.

49. The reader of claim 45, further comprising:  
a control unit including a processor modified with a software subsystem.

50. The reader of claim 46, further comprising:  
a control unit including a processor modified with a software subsystem.  
20 51. The reader of claim 49, wherein said processor includes means for detecting the reflection signal and for generating an output signal indicative of an amount of analyte in response thereto.

52. The reader of claim 50, wherein the software comprises a decision-support system.

25 53. The reader of claim 52, wherein the decision-support system is a neural net.

54. A method for reading determining a risk or identifying a condition associated with the presence of fetal fibronectin in a cervicovaginal sample, comprising:  
30 obtaining a cervicovaginal sample and reacting it with an antibody on a lateral flow test device to produce a stripe on the test device indicative of the presence of fFN in the sample;

-81-

reading the result with a reflectance reader that comprises a reader head by scanning the reader head to a first position over the test device;

determining a first amount of light reflected from the surface comprising the image;

5        illuminating the surface for light of a first wavelength, and determining a second amount of light reflected from the surface;

illuminating the surface for light of a second wavelength, and determining a third amount of light reflected from the surface; and

determining the amount of FFN in the sample.

10       55. The method of claim 54, further comprising, correlating the amount with the risk of developing a pregnancy related condition, with the presence of the condition, or with fertility status.

56. The method of claim 55, wherein the condition is selected from the group consisting of ectopic pregnancy, infertility, preterm labor, pre-eclampsia,  
15       imminent delivery, term induction and fetal membrane rupture and infections of concern during pregnancy that may comprise the pregnancy or harm the newborn, including, for example, ascending genital infections such as chlamydia or herpes simplex virus.

57. A method of classifying an image, comprising:

20       reducing the image to a set of derived parameters that are can be used to reconstruct the image within a specified degree of tolerance;

inputting the derived parameters into a classification means; and

determining the classification of the image based on the output of the classification means.

25       58. The method of claim 57, wherein the classification means is a neural network.

59. The method of claim 57, wherein the means of reducing the image to a set of derived parameters comprises:

defining a mathematical function containing a plurality of parameters

30       representative of the image; and

-82-

optimizing the parameters of the mathematical function using a numerical technique that minimizes the error between the image and a reconstruction of the image using the mathematical function.

60. The method of claim 57, wherein the means of reducing the  
5 image to a set of derived parameters comprises:

inputting the image to a trained neural network, wherein the inputs to the network represent the image, the network comprises a hidden layer where the number of hidden elements is smaller than the number of inputs to the network, and the outputs of the network represent the reconstruction of the  
10 image; and

setting the derived parameters to the output values of the trained neural network.

61. The method of claim 57, wherein the means of reducing the image to a set of derived parameters comprises:  
15 defining a neural network wherein the inputs to the network are the coordinates of a point in the image, a hidden layer contains a plurality of elements, and the output of the network represents the reconstruction of the associated point in the image;

training the neural network so that the error between the network output  
20 and the image are minimized for all points in the image; and

setting the derived parameters to the weights of the hidden layer of the trained neural network.

62. A method for determining results from a test strip, comprising:  
(a) scanning the test strip in a reflectance reader to obtain a scanned  
25 image, wherein the signal is indicative of the presence of the analyte; and  
(b) processing the data obtained from the reflectance signals using data processing software employing data reduction and curve fitting algorithms and/or a trained neural network to convert the reflectance signal obtained from reading the test strip into a data indicative of the test results presence or  
30 absence or a threshold concentration of analyte in a sample by a process that comprises:

-83-

reducing the image to a set of derived parameters that are can be used to reconstruct the image within a specified degree of tolerance;

inputting the derived parameters into a classification means; and

determining the classification of the image based on the output of the

5 classification means.

63. The method of claim 62, wherein the classification means is a neural network.

64. The method of claim 62, wherein the means of reducing the image to a set of derived parameters comprises:

10 defining a mathematical function containing a plurality of parameters representative of the image; and

optimizing the parameters of the mathematical function using a numerical technique that minimizes the error between the image and a reconstruction of the image using the mathematical function.

15 65. The method of claim 62, wherein the means of reducing the image to a set of derived parameters comprises:

inputting the image to a trained neural network, wherein the inputs to the network represent the image, the network comprises a hidden layer where the number of hidden elements is smaller than the number of inputs to the  
20 network, and the outputs of the network represent the reconstruction of the image; and

setting the derived parameters to the output values of the trained neural network.

25 66. The method of claim 62, wherein the means of reducing the image to a set of derived parameters comprises:

defining a neural network wherein the inputs to the network are the coordinates of a point in the image, a hidden layer contains a plurality of elements, and the output of the network represents the reconstruction of the associated point in the image;

30 training the neural network so that the error between the network output and the image are minimized for all points in the image; and

-84-

setting the derived parameters to the weights of the hidden layer of the trained neural network.

67. The method of claim 62, wherein the processing of data process, comprises:

- 5 (i) reducing the raw reflectance data;
- (ii) plotting the reduced data to generate a second image of the data;
- (iii) expressing the second image as a polynomial mathematical function to generate parameters that define this image; and
- 10 (iv) comparing the parameters to parameters generated from a reference sample, whereby a positive, negative or quantitative result is obtained.

68. The method of claim 62, wherein the data is processed by a process, comprising:

- 15 (i) optionally correcting the reflectance readings to correct for light leakage;
- (ii) reducing the raw reflectance data using a radiometric formula;
- (iii) generating an second image of the test data by plotting the reduced data;
- 20 (iv) expressing the second image as a polynomial mathematical function, and generating parameters that define the image;
- (v) comparing the scanned image and second image by solving the linear regression through the curves;
- (vi) validating the parameters obtained from the curve-fitting
- 25 results to obtain a validated result; and
- (vii) classifying the validated result as positive or negative by comparing peak heights of a clinical sample to reference samples.

69. The method of claim 68, wherein the data is processing process, further comprises:

- 30 (viii) inputting the validated result into a decision-support system to generate a medical diagnosis or risk assessment.

-85-

70. The method of claim 62, wherein the data is processing process, further comprises:

(viii) inputting the result into a decision-support system to generate a medical diagnosis or risk assessment.

5        71. The system of claim 3, wherein the test strip further comprises a symbology.

72. The system of claim 71, wherein the symbology comprises information associated with the performance or results of the assay.

73. The system of claim 71, wherein the symbology is a bar code.

10       74. The system of claim 71, comprising further comprising a reader for reading the symbology.

75. The system of claim 71, wherein the reader for analyzing data from the test is also adapted to read the symbology on the test device.

15       76. The system of claim 71, further comprising software for decoding the symbology.

77. The reader of claim 29, wherein the assay is an immunoassay.

78. The reader of claim 29, that is adapted for reading an assay test strip and a symbology that is imprinted, engraved or affixed on the test strip.

20       79. The method of claim 37, wherein the surface comprises an immunoassay test strip.

80. The method of claim 40, wherein the assay strip comprises a symbology that is associated with data resulting to the assay, results thereof reagents or test sample, and the method further comprises reading the symbology.

25       81. The system of claim 75, wherein the adaptation permits the reader to adjust to its height relative to the test device.

82. A reflectance reader, comprising:

a reader head comprising:

a reader head body;

30       two light emitting diodes;

a first fiberoptic bundle optically coupled to the first light emitting diode;

-86-

a second fiberoptic bundle optically coupled to the second light emitting diode;

a photodetector;

a third fiberoptic bundle optically coupled to the light

5 photodetector;

an aperture in the reader head body;

a plurality of fiberoptic conductor ends arranged in a sigmoidal distribution in the aperture, a first portion of the fiberoptic conductor ends being of fiberoptic conductors of the first fiberoptic bundle, and a second portion of  
10 the fiberoptic conductor ends being of fiberoptic conductors of the second fiberoptic bundle.

83. The reader of claim 82 that is adapted for reading a symbology on a test device inserted into the reader.

84. The reader of claim 83, wherein the height of the reader head  
15 relative to the test device is adjustable.

85. The reader of claim 83, further comprising software for decoding the symbology.

86. The reader of claim 83, wherein the symbology is a bar code.

87. A method of developing and using a control for any assay system,  
20 comprising:

analyzing a plurality of test runs of the assay and obtaining results of the test runs;

classifying the results by type of result; and  
identifying a pattern representative of or predictive of each type of result.

88. The method of claim 87, further comprising,  
25 performing the test, and identifying the pattern contained within the results; and

classifying the test results based upon the identified pattern.

89. The method of claim 87, wherein the test results are classified as  
30 invalid based upon deviation from the identified pattern.

90. The method of any of claims 87-90, wherein classification is effected by pattern recognition means.



-87-

91. The method of any of claims 87-90, wherein the pattern recognition means is a curve fitting procedure or is a neural network.

91. The method of claim 87, wherein the pattern is curve

91. The method of claim 87, comprising:

5 fitting the data obtained from the assay to a predetermined mathematical function based on expected results for the assay; and  
accepting or rejecting the data based on the quality of the fit between actual and expected data.

10 92. The method of claim 62, wherein step (b), the processing of data process, comprises:

(i) reducing the raw reflectance data;

(ii) plotting the reduced data to generate a second image of the data;

15 (iii) expressing the second image as a polynomial mathematical function to generate parameters that define this image;

(iv) validating the parameters obtained, wherein validation is accomplished by fitting the data obtained from the assay to a predetermined mathematical function based on expected results for the particular assay; and  
20 accepting or rejecting the data based on the quality of the fit between actual and expected data; and

(v) comparing the parameters to parameters generated from a reference sample, whereby a positive, negative or quantitative result is obtained.

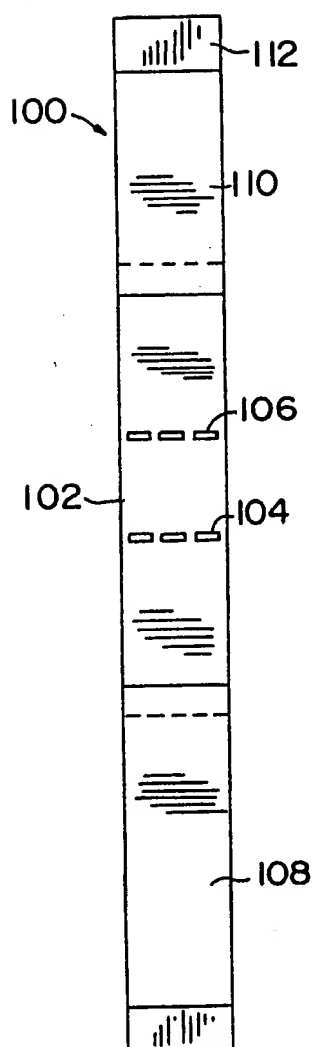


FIG. 1A

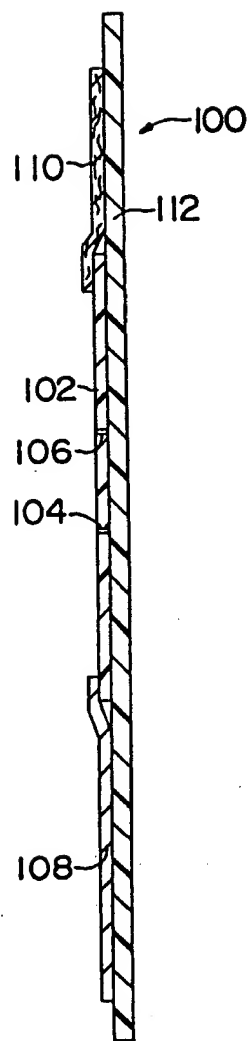


FIG. 1B

2/15

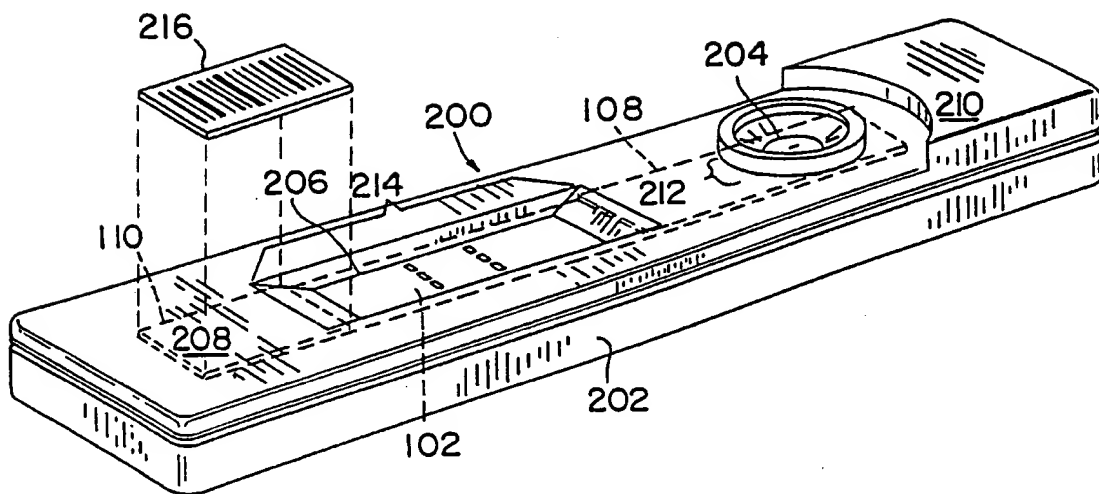


FIG. 2A

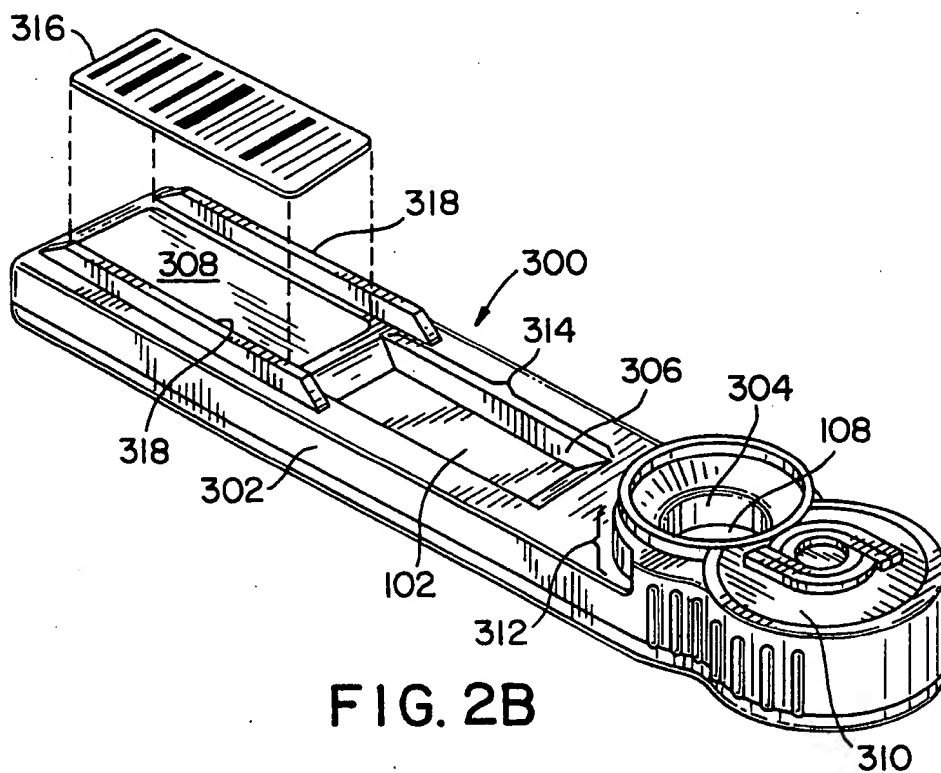


FIG. 2B

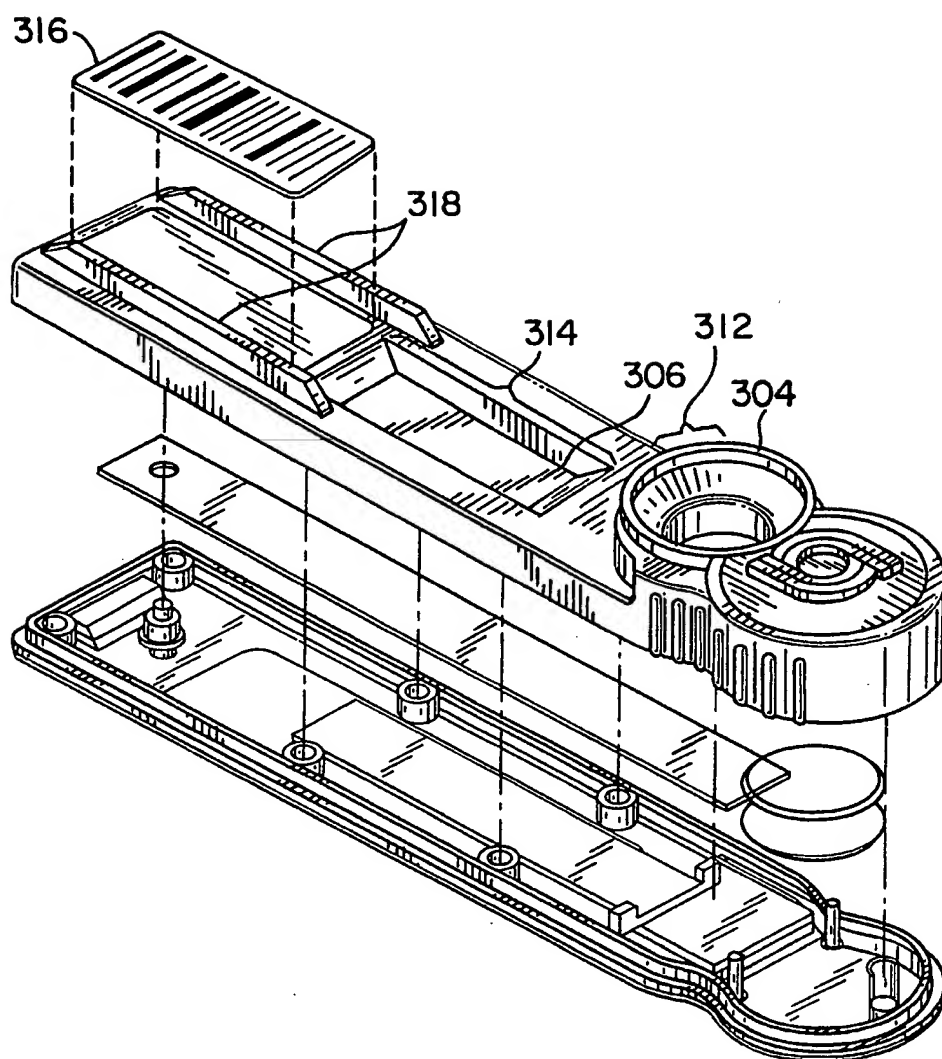


FIG. 3

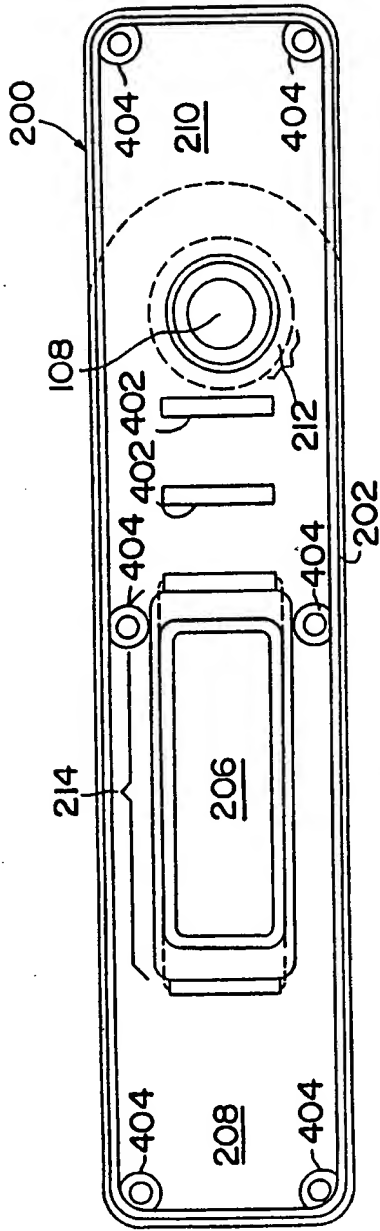


FIG. 4

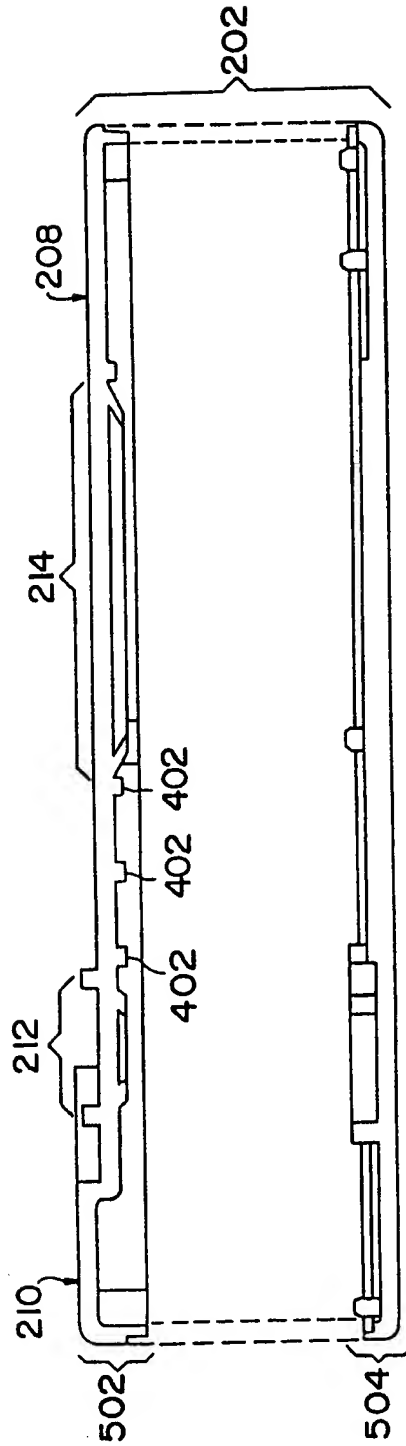


FIG. 5

5/15

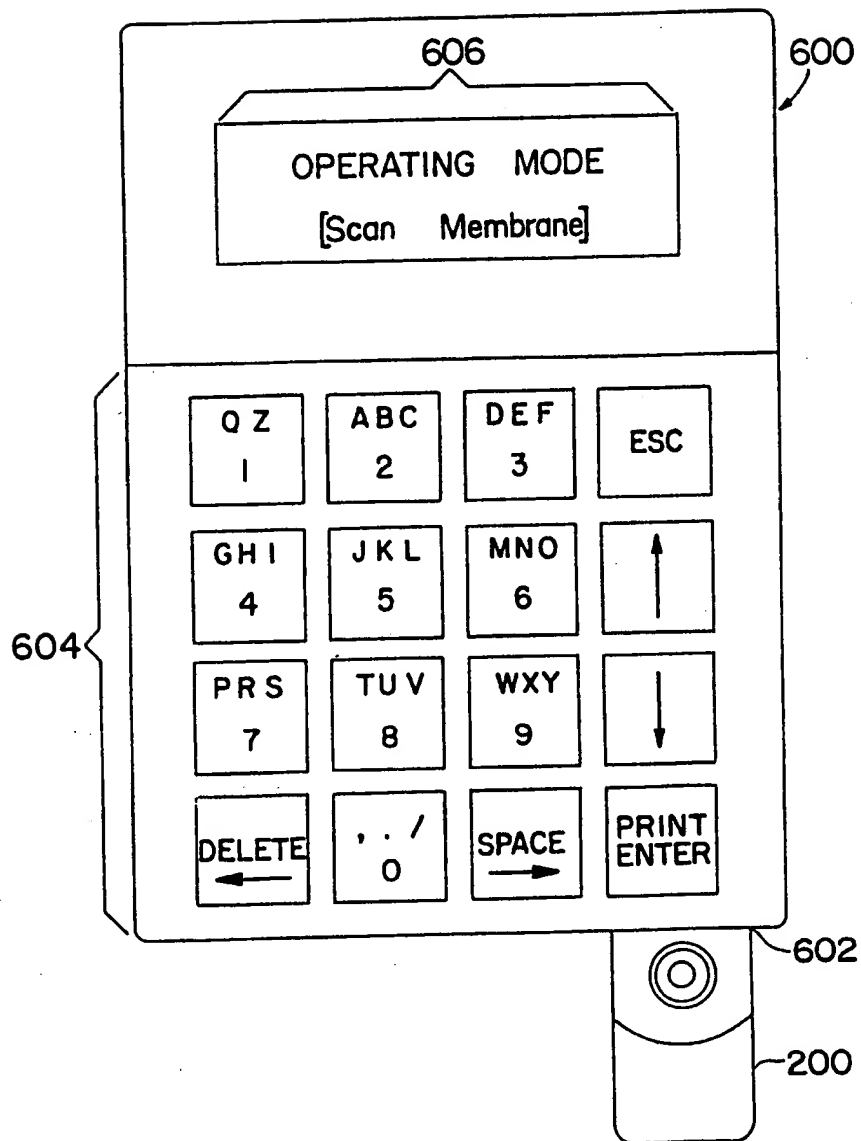


FIG. 6

6/15

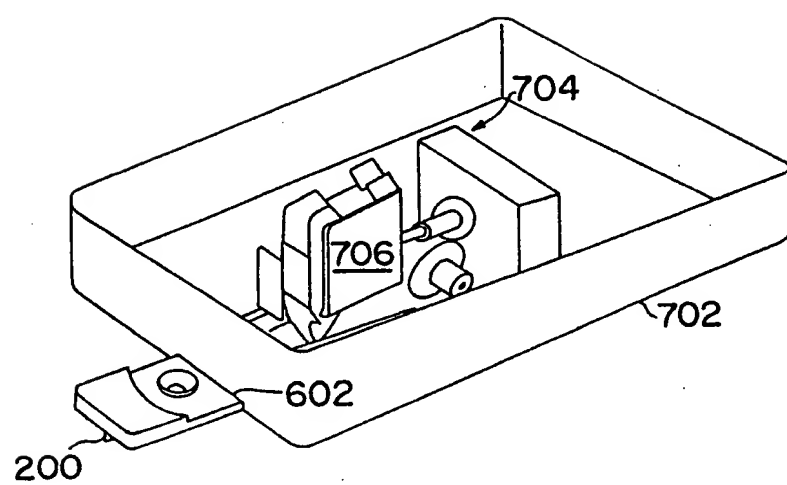


FIG. 7

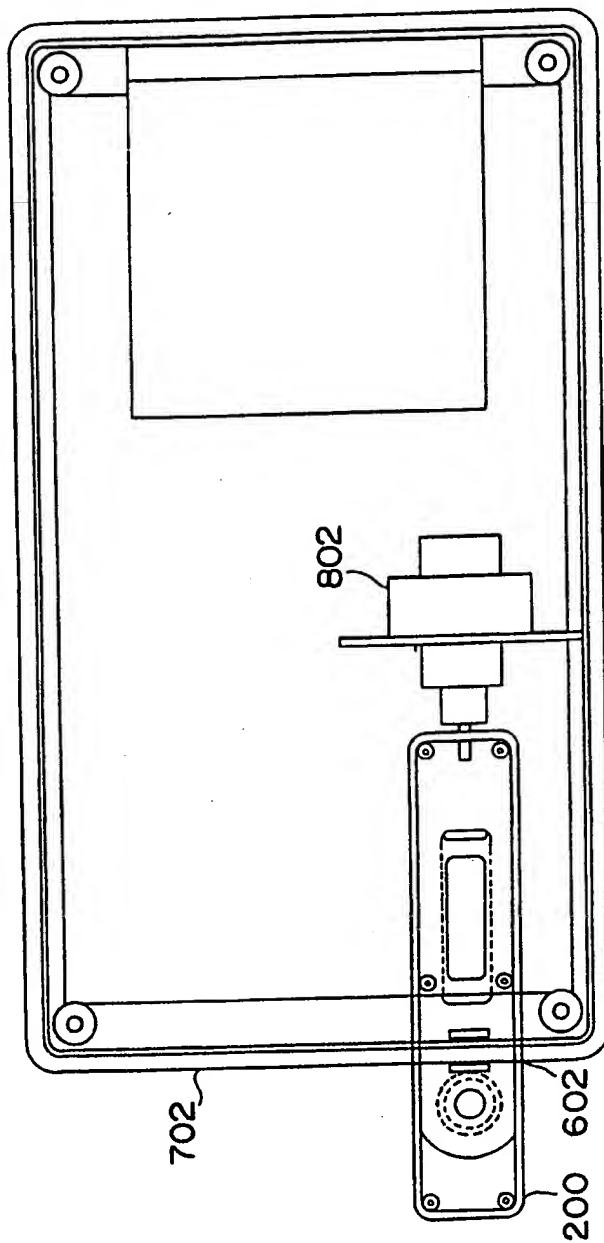


FIG. 8



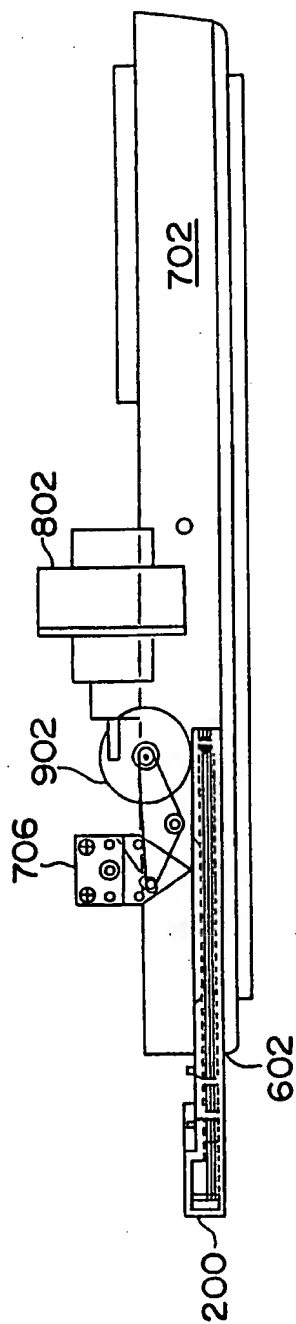


FIG. 9

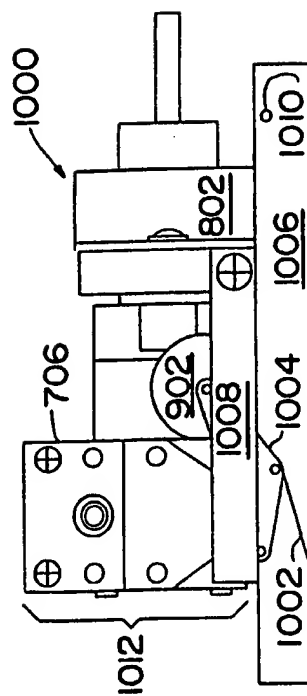


FIG. 10

9/15

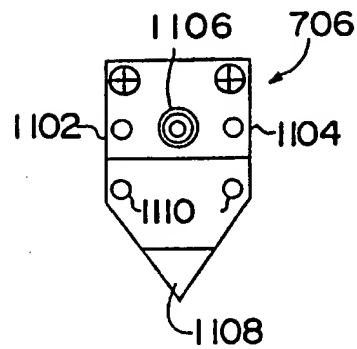


FIG. 11

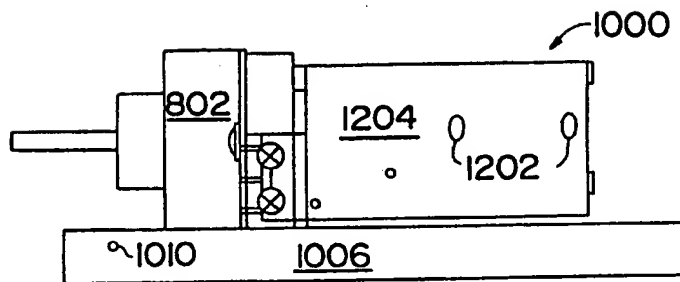


FIG. 12




FIG. 13

10/15

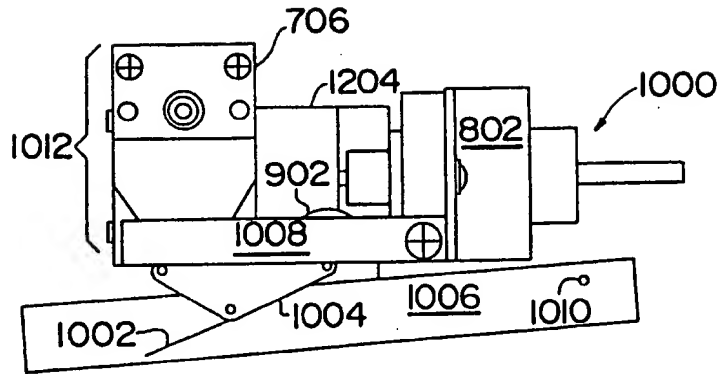


FIG. 14

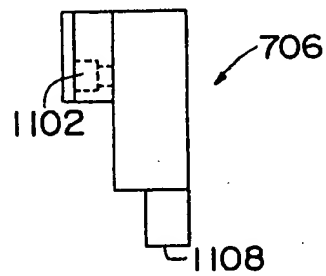


FIG. 15

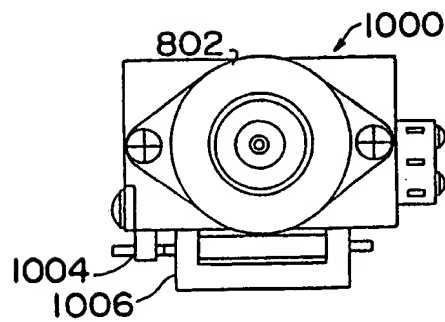


FIG. 16

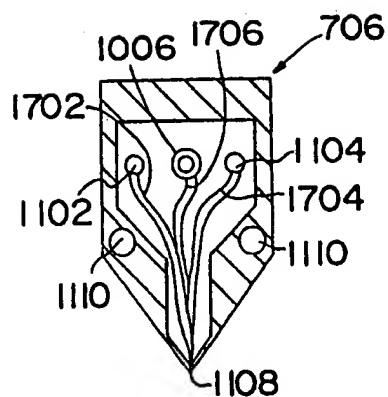


FIG. 17

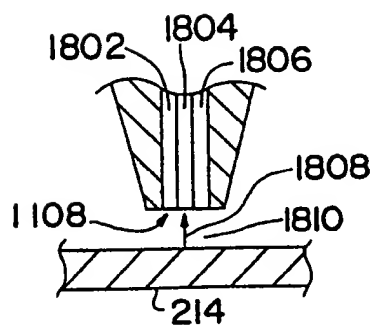


FIG. 18

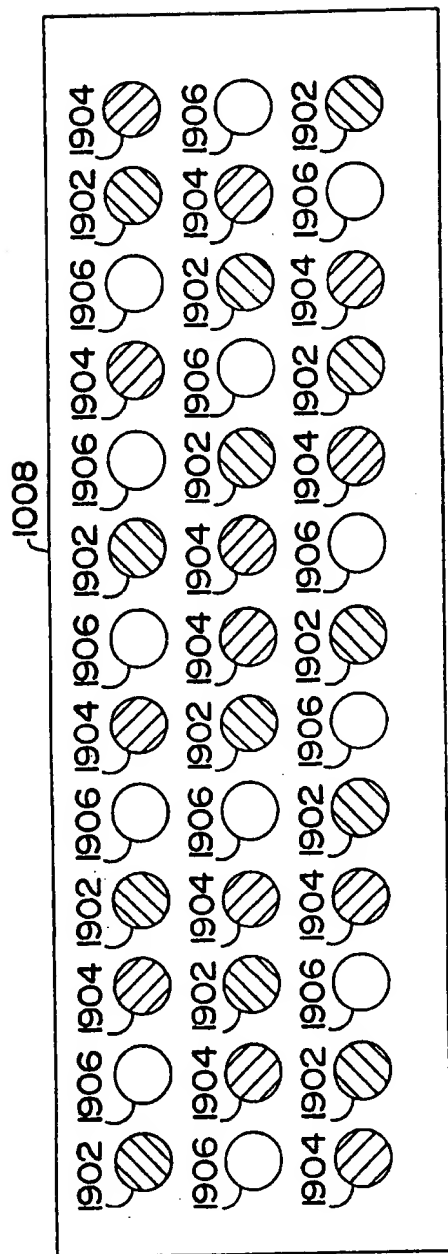


FIG. 19

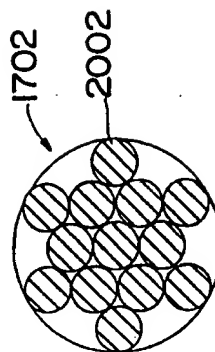


FIG. 20

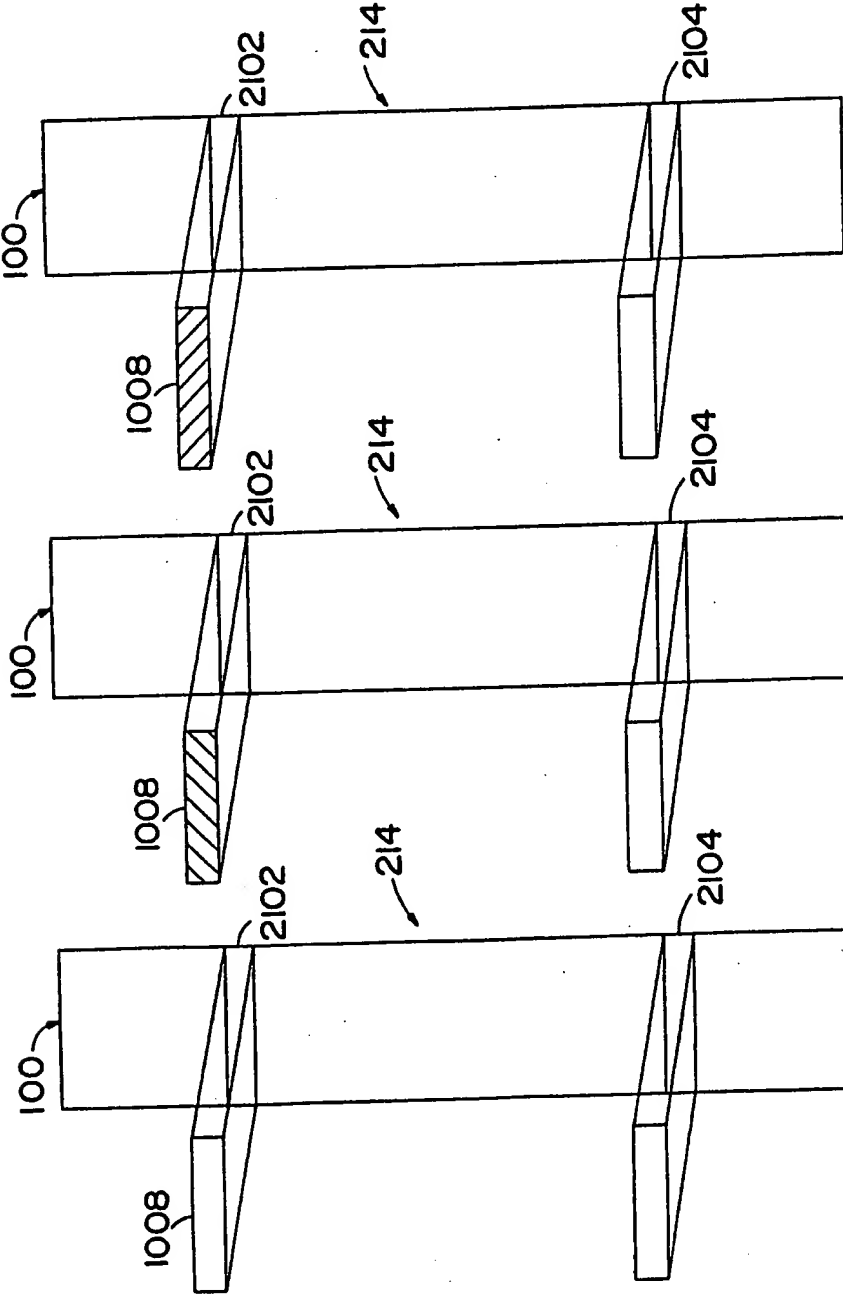


FIG.23

FIG.22

FIG.21

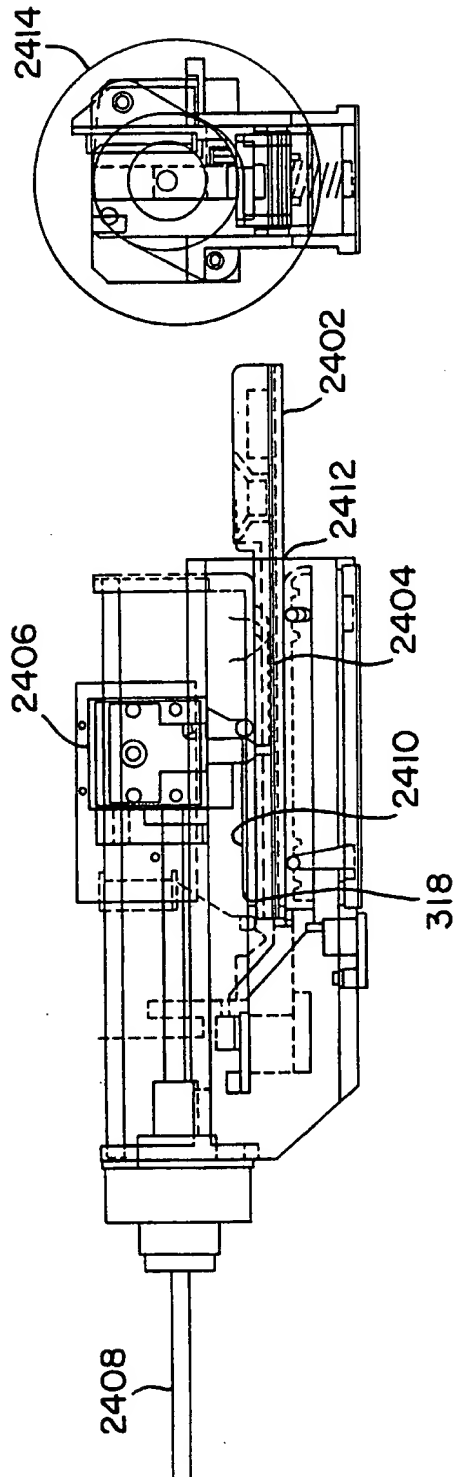


FIG. 24

15/15



FIG. 25



# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 99/02282

## A. CLASSIFICATION OF SUBJECT MATTER

IPC 6 G06F19/00 G01N21/00

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 6 G06F G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	WO 94 27490 A (BASE TEN SYSTEMS INC) 8 December 1994 (1994-12-08)	1
Y	page 1, line 1 - page 7, line 25	2-4
A	---	87
X	EP 0 644 414 A (HITACHI LTD) 22 March 1995 (1995-03-22)	57, 58
Y	column 3, line 22 - column 5, line 56	19, 62
A	---	54
Y	US 5 304 468 A (PHILLIPS ROGER ET AL) 19 April 1994 (1994-04-19)	2-4, 19,
A	column 3, line 48 - column 11, line 32; figures 1-4	62
	---	28, 44,
A	EP 0 387 630 A (MILES INC) 19 September 1990 (1990-09-19)	54, 82, 87
	page 4, line 30 - page 5, line 7	87
	---	
	-/--	



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

### \* Special categories of cited documents :

"A" document defining the general state of the art which is not considered to be of particular relevance

"E" earlier document but published on or after the international filing date

"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O" document referring to an oral disclosure, use, exhibition or other means

"P" document published prior to the international filing date but later than the priority date claimed

"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.

"&" document member of the same patent family

Date of the actual completion of the international search

7 July 1999

Date of mailing of the international search report

13/07/1999

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2  
NL - 2280 HV Rijswijk  
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,  
Fax: (+31-70) 340-3016

Authorized officer

Schenkels, P

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/US 99/02282

## C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	<p>US 5 321 492 A (DETWILER PAUL S ET AL)  14 June 1994 (1994-06-14)  column 1, line 13 - column 3, line 9  -----</p>	<p>1,28,44,  54,82</p>

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 99/02282

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
WO 9427490 A	08-12-1994	US 5594637 A	14-01-1997
		AT 172561 T	15-11-1998
		AU 7015694 A	20-12-1994
		CA 2163082 A	08-12-1994
		DE 69414108 D	26-11-1998
		DE 69414108 T	06-05-1999
		EP 0700542 A	13-03-1996
		JP 9500290 T	14-01-1997
		US 5492117 A	20-02-1996
		US 5796759 A	18-08-1998
EP 0644414 A	22-03-1995	JP 7055688 A	03-03-1995
		JP 7113738 A	02-05-1995
		US 5715182 A	03-02-1998
US 5304468 A	19-04-1994	US 5179005 A	12-01-1993
		US 4935346 A	19-06-1990
		AU 3375789 A	02-11-1989
		CA 1337682 A	05-12-1995
		DK 204289 A	29-10-1989
		GR 89100286 A,B	31-01-1990
		JP 1318963 A	25-12-1989
		PT 90386 A,B	10-11-1989
		US 5426032 A	20-06-1995
		US 5563042 A	08-10-1996
		US 5843692 A	01-12-1998
		AT 96179 T	15-11-1993
		AT 174687 T	15-01-1999
		AT 172538 T	15-11-1998
		AT 172499 T	15-11-1998
		AU 603821 B	29-11-1990
		AU 7675887 A	18-02-1988
		CA 1301604 A	26-05-1992
		CN 1011919 B	06-03-1991
		CN 1050930 A,B	24-04-1991
		CN 1116307 A	07-02-1996
		DE 3752229 D	26-11-1998
		DE 3752229 T	02-06-1999
		DE 3752230 D	26-11-1998
		DE 3752230 T	06-05-1999
		DE 3752241 D	28-01-1999
		DE 3752241 T	17-06-1999
		DE 3787851 D	25-11-1993
		DE 3787851 T	21-04-1994
		DK 91594 A	05-08-1994
		DK 157092 A	29-12-1992
		DK 157192 A	29-12-1992
		DK 419187 A	14-02-1988
		EP 0256806 A	24-02-1988
		EP 0479394 A	08-04-1992
		EP 0473241 A	04-03-1992
		EP 0656423 A	07-06-1995
		EP 0816849 A	07-01-1998
		ES 2046985 T	16-02-1994
		ES 2126562 T	01-04-1999
		ES 2121766 T	16-12-1998
		ES 2124490 T	01-02-1999
		FI 873356 A,B,	14-02-1988

# INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/US 99/02282

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 5304468	A		FI 942818 A,B,	14-06-1994
			FI 951491 A	29-03-1995
			GR 3026514 T	31-07-1998
			IE 64442 B	09-08-1995
			JP 2589053 B	12-03-1997
			JP 7067698 A	14-03-1995
			JP 2107205 C	06-11-1996
-----				
EP 0387630	A	19-09-1990	AU 622293 B	02-04-1992
			AU 5122190 A	29-11-1990
			CA 2010165 A	13-09-1990
			JP 2278142 A	14-11-1990
-----				
US 5321492	A	14-06-1994	AT 171273 T	15-10-1998
			AU 653105 B	15-09-1994
			AU 4422093 A	14-04-1994
			CA 2100735 A	08-02-1994
			DE 69321114 D	22-10-1998
			DE 69321114 T	04-03-1999
			EP 0636878 A	01-02-1995
			ES 2121037 T	16-11-1998
			JP 6213806 A	05-08-1994
-----				